


Omni 4

Logic

Analyzer

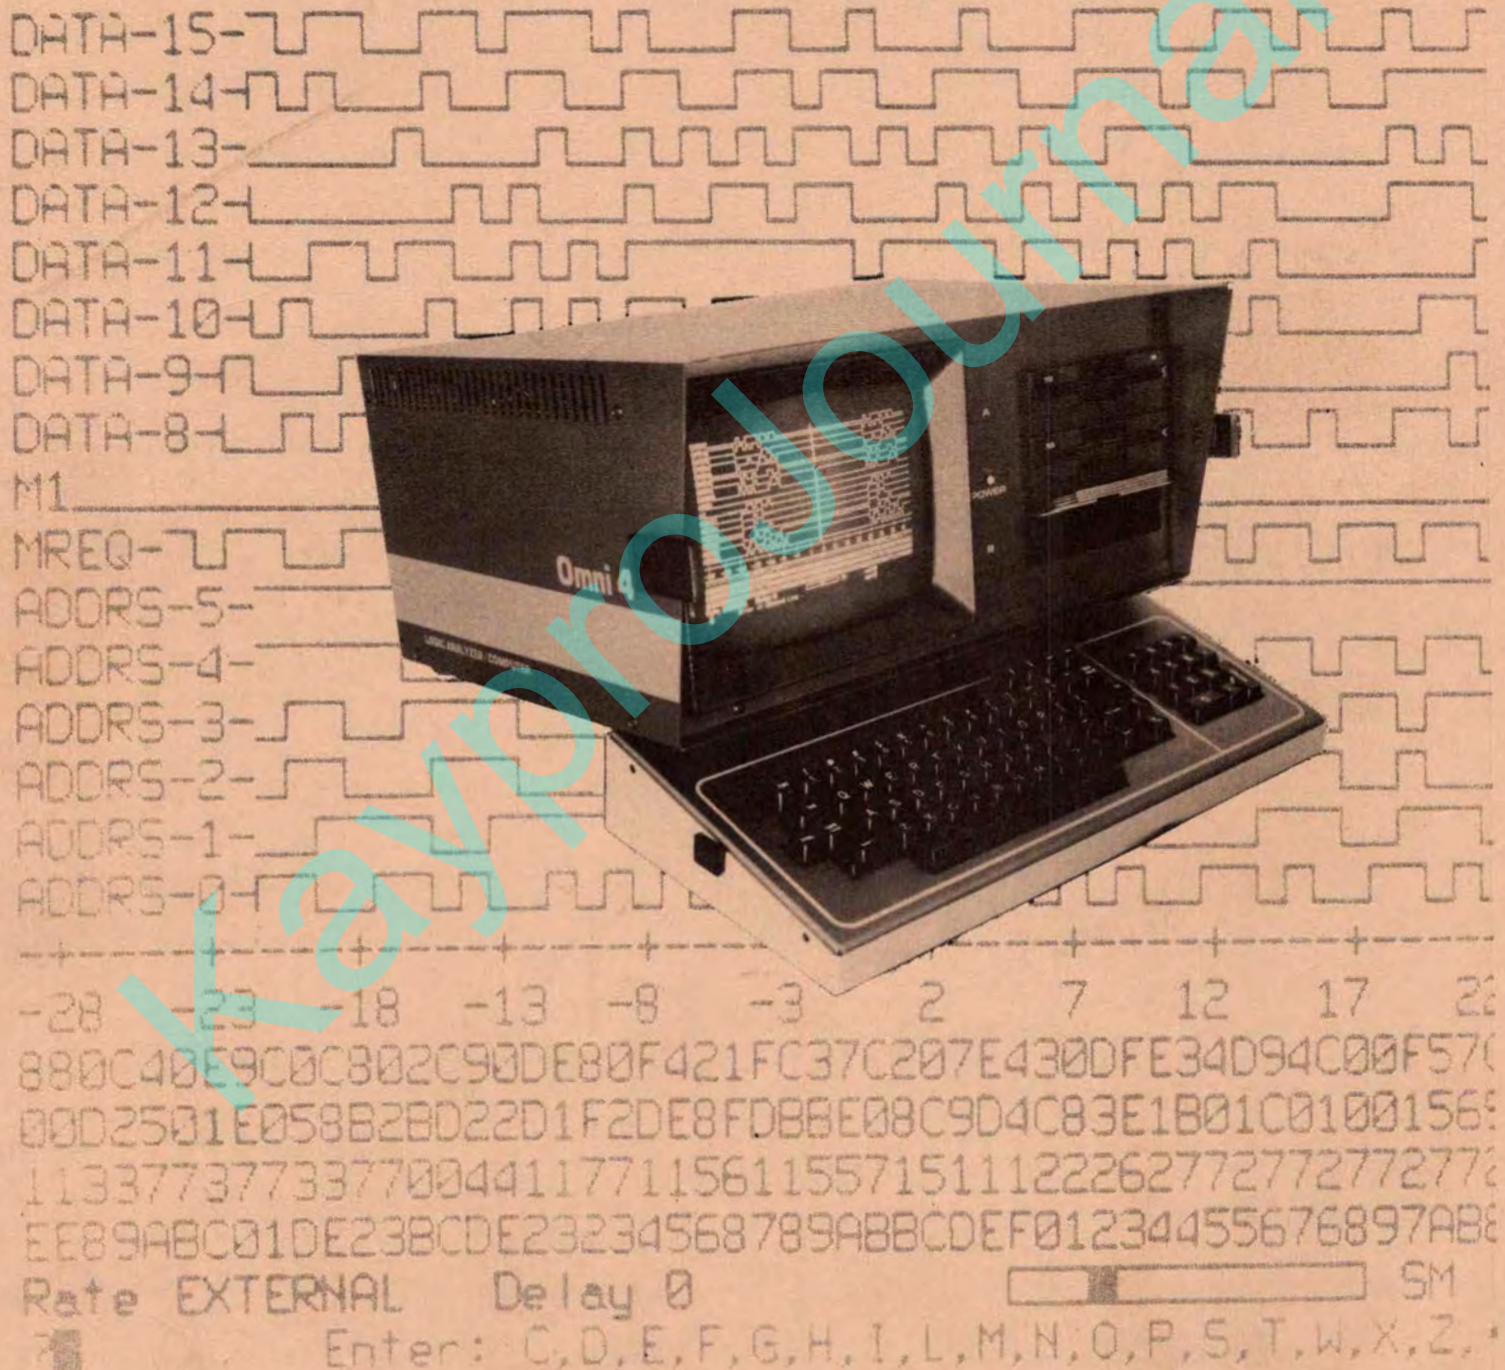

Omni 4
Logic Analyzer
Operating Manual

OmniLogic, Inc.
P.O.Box 87
Renton, WA 98057
(206) 271-2000

(c) 1985 OmniLogic, Inc. All rights reserved. May not be copied in whole or in part without written permission.

Manual Part No. 6000-6
Rev. D

TABLE OF CONTENTS

	<u>Page</u>
I. Preliminary	
1. Cautionary Warning and Warranty	1-1
2. Introduction	2-1
3. Specifications	3-1
4. Unpacking	4-1
5. Turn-on Procedure	5-1

II. Logic Analyzer Operation

6. Basic Operation	6-1
7. Input Probes and Output Signals	7-1
8. Menus and Commands	8-1
9. Help Pages	9-1
10. Trigger Condition Setup Menu	10-1
11. Options Menu	11-1
12. Go and Start Data Collection	12-1
13. Waveform Display	13-1
14. Edge Display	14-1
15. Name Command	15-1
16. Interval Calculation	16-1
17. Dump Display	17-1
18. Correlation	18-1
19. Matrix Display	19-1
20. Locate	20-1
21. File Operations	21-1
22. Instruction Disassembly	22-1
23. Histogram Display	23-1
24. Signature Analysis	24-1
25. Print Command	25-1
26. Theory of Operation	26-1
27. Applications	27-1
28. Advanced Applications	28-1
29. 32 Channel Expansion Module (Model 3032)	29-1
30. Pattern Generator (Model 3010)	30-1


Kaypro Journal

III. Appendices

- A. Quick Start
- B. Reference Card

A-1

B-1

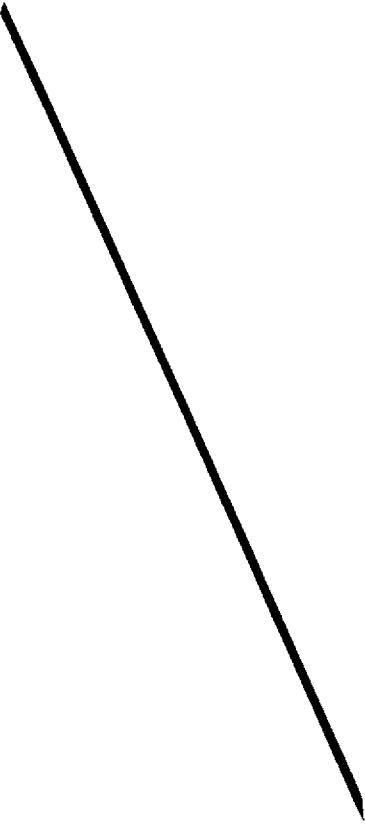

1. CAUTIONARY WARNING AND WARRANTY

1.1 CAUTIONARY WARNING

The logic analyzer functions of the Omni Series are designed for use only by qualified technical personnel trained to work on electronic circuitry that is in a power-on condition. Such circuitry may have hazardous voltages present; the operator must have a knowledge of electronic circuit operation, accepted maintenance procedures, and appropriate safety practices for the circuitry being tested.

1.2 LIMITED WARRANTY

OmniLogic, Inc., warrants each new system against defects in material or workmanship for a period of ninety days from date of delivery to the original customer. The Logic Analyzer Printed Circuit Board has a warranty period of one year. Fuses, probes, and probe tips are excluded from this warranty. This warranty is specifically limited to the replacement or repair of any defects, without charge, when work is authorized or unit is returned to OmniLogic, Inc., 350 Sunset Blvd N., Renton, WA 98055, transportation charges prepaid. This express warranty excludes all other warranties, expressed or implied, and IN NO CASE SHALL THE LIABILITY OF OMNILOGIC, INC., EXCEED THE PURCHASE PRICE OF THE UNIT. OMNILOGIC, INC., SHALL NOT BE MADE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES. No liability is assumed for damage due to accident, abuse, lack of reasonable care, loss of parts, unauthorized service, or subjecting the instrument to faulty peripherals or input values exceeding specified limits.

2. INTRODUCTION

This manual describes the operation of OmniLogic, Inc.'s Logic Analyzers. The purpose of the manual is to enable you to use the Omni analyzer to make digital measurements most effectively. The Omni is designed for maximum user convenience so that your attention will be on the circuit you are testing, rather than on the instrument itself.

Menus and on-line Help Page explanations make the Omni extremely easy to use. Every screen display includes a prompt line at the bottom which gives you the allowable commands. A label on the keyboard also lists the most often used commands. Little training or reference to other materials are needed to use the instrument effectively. Most of the material in this manual, in fact, is on-line and available to you with a few keystrokes; the Omni, itself, will teach you most of what you need to know in order to use it.

This manual covers only the Logic Analyzer functions. Use of the Omni as a CP/M computer is described in the computer manuals packed with the unit.

This manual has a section devoted to each command, and covers the operation of the Omni analyzer in detail. The last section, "Quick Start", leads you through the functions and commands, beginning with turn-on. If you have never used the Omni before, we suggest you start with the Quick Start section (Appendix A) and go step-by-step through the Omni's functions. Due to software improvements, there may be slight differences between photos in this manual, the descriptions, and your unit.

The information in the Help Pages in your Omni may vary slightly from that given here; if so, check the revision date to make sure that you have the latest version.

Rev. D

3. OMNI SPECIFICATIONS*

3.1 LOGIC ANALYZER DATA COLLECTION CHARACTERISTICS

Sample Rates	
Internal Clock	
Available periods	50, 100, 200, 500ns 1, ... 32768us
External Clock	
Minimum period	50ns
Maximum period	unlimited
Clock stable prior to active edge	35ns
Clock Qualify	
Setup	30ns
Hold	0ns
Number of samples collected	1000
Trigger point	16th, 32nd, ... 992nd sample
Delay between event trigger to data collection	0 to 34 seconds
Data Channels F through 0	
Data stable prior to active edge of clock	35ns
Data stable after active edge of clock	0ns
Glitch Channels 3 through 0	
Glitch definition	2 or more data transitions in 1 sample period
Minimum detectable pulse	10ns

3.2 TRIGGER CONDITIONS

Data functions	AND/OR/NOT on data
Glitch functions	AND/OR/NOT with data

*Specifications are subject to change without notice.

Latched (synchronous) mode	
Setup	30ns
Hold	0ns
Unlatched (asynchronous) mode	
Minimum event duration	15ns
External Trigger duration	25ns
External Trigger Qualify	
Minimum active during event	25ns
Active after	0ns
Timeout mode	
Duration between events	16us to 34sec
Repeat until reference memory correlated or not correlated	

3.3 DISPLAY MODES

Waveform format	
Sample window	80 to 1000 samples, scrollable
Number of channels	1 to 16 channels
Edge format	
Sample window	80 to 1000 samples, scrollable
Number of channels	1 to 16 channels
Dump format	
Sample window	252 binary, 231 octal 232 unsigned decimal 232 signed decimal 336 hexadecimal all scrollable
Number of channels	1 to 16
Matrix format	
Sample window	1 to 1000 samples
Number of channels	2 to 8
Display matrix	16 rows X 16 columns
Instruction Disassembly format	
Sample window	13 scrollable
Number of channels	4, 8, or 16
Processors supported	Z-80, 8085, 8048 family and user-definable

Specifications are subject to change without notice.

Signature format
 Sample window 2 to 1000 samples
 Number of channels 1 to 14 simultaneous

3.4 UTILITY CAPABILITIES

Pattern Search 1 to 16 bit maskable
 1 to 6 sample sequence

Interval Calculation Time and sample number
 between cursor
 and/or 2 events

Correlation 1 to 1000 samples
 1 to 1000 start skew
 1 to 16 channel tolerance
 1 to 1000 sample
 error allowance

Channel Labels 1 to 15 characters
 per channel

Printer Output Any display on CRT
 and multiple
 sequential displays

File Operations Save and recover set-up
 and/or data

Help Pages Built-in explanations
 and examples at all
 steps of operation

Extensive built-in tests

3.5 PROBE CHARACTERISTICS

<u>Pin</u>	<u>Left Pod</u>	<u>Right Pod</u>	<u>Suggested Lead Color</u>
1	Clock	Clock Qualifier	Yellow/White
2	D0	D8	Black
3	D1	D9	Brown
4	D2	D10	Red
5	D3	D11	Orange
6	D4	D12	Yellow
7	D5	D13	Green
8	D6	D14	Blue
9	D7	D15	Violet
10	Trigger	Trigger Qualifier	Red/White
11	Ground	Ground	Green/White

Specifications are subject to change without notice.

Minimum detectable pulse	10 nanoseconds
Maximum voltage limits	-0.5V, +5.5V
Input impedance	1 megohm
Logic level transition to low level	
TTL probes	0.8V
CMOS probes	1.0V
Logic level transition to high level	
TTL probes	2.0V
CMOS probes	3.5V

Specifications are subject to change without notice.

CP/M COMPUTER*

CPU	Z-80A System
RAM	64K Bytes
Mass storage	Omni II - 380 Kbytes via dual 5-1/4 inch, single sided, double density floppy disk drives Omni 4 - 780 Kbytes via dual 5-1/4 inch, double sided, double density floppy disk drives
Disks recommended	Omni II - single sided 5-1/4 inch floppy disks (Maxell MD1-D) Omni 4 - double sided 5-1/4 inch floppy disks (Maxell MD2-D)
Keyboard	Full ASCII keyboard with numeric pad and cursor control keys, detachable. Keys are programmable.
Display	9 inch, 24 row x 80 column 8 x 11 pixel character Omni II and 4 - green phosphor
Graphics	Omni 4 - 160 x 100 pixels
I/O connections	RS-232C serial port (Omni 4 has two serial ports) "Centronics" parallel port
Modem (Omni 4 only)	300 Baud, full or half duplex, auto dial/auto answer
Real Time Clock (Omni 4 only)	Resolution to .0001 second, 5-year lithium battery backup

*Specifications are subject to change without notice.

Rev. D

4. UNPACKING

If there is damage to the inner carton, inspect the Omni carefully. If the Omni is damaged, call us immediately at (206) 271-2000 for further instructions.

Set the Omni on a firm surface. The keyboard is attached to the main unit by clamps at the right and left sides. The keyboard cable may be packed between the keyboard and main unit. The Omni 4 provides a storage area for the probes below the disk drives, and the probes and probe leads are packed there. There is also a convenient disk storage area just below the drives.

The Omni logic analyzer disks and the CP/M Operating System Disk are packed separately from the other disks and manuals, which are in a single large flat package within the Logic Analyzer carton.

Remove the remaining items from the carton, along with the System Checklist. Verify that you have received everything on the Checklist. If there are any items missing compared to the Checklist enclosed with the unit, please call and let us know.

Table 4-1 on the next page shows a typical checklist.

Table 4-1 TYPICAL SYSTEM CHECKLIST

NOTE: This list is provided here as an illustration only. The items included in your system may be different. Use the correct System Checklist enclosed with your unit to verify that your shipment is complete.

<u>Item No.</u>	<u>Qty.</u>	<u>Description</u>
1	2	Omni Logic Analyzer Disks (master and working copy)
2	1	CP/M Operating System Disk
3	1	Software Package - package of manuals and disks
4	1	Operating Manual (this manual)
5	1	Main Unit with Power Cord
6	1	Keyboard
7	1	Keyboard Cable
8	2	Cables and Pods each ribbon cable is 36" long and has a pod at one end
9	2	Package of 11 Leads with 11 Clips 6" leads, ganged together

Rev. D

5. TURN-ON PROCEDURE

5.1 INTRODUCTION

Now that you have the Omni unpacked, you can set it up and try it out. The Omni may be used as either a Z-80 based computer with the CP/M operating system or as a logic analyzer for probing the operation of digital circuits.

The Omni should be used to test digital equipment only by qualified technical personnel (see "Cautionary Warning", Section 1).

The Omni is intended to operate from an 120 volt AC, 60 Hz power source as marked on the rear panel. The Omni is grounded through the grounding conductor of the power cord. To avoid electrical shock, plug the power cord into a properly wired receptacle before connecting to the input or output terminals. A protective ground connection by way of the grounding conductor in the power cord is essential for safe operation.

We also recommend that you use the Omni only on a safe technician's test bench when testing digital circuits. That means: 1) A bench or table on which any metal parts you are likely to come in contact with are grounded. Then if a conductor carrying high voltage comes in contact with the bench, it will not make the bench itself "hot" and a hazard to you. 2) A nonconductive surface should be on the floor in front of the bench for you and your chair to stand on. Thus, if you do inadvertently come in contact with a hazardous voltage circuit, there is no current path through you to ground.

OPERATOR SAFETY COMES FIRST

If necessary, ground your bench now before proceeding further.

CAUTION

Both the Omni main unit and the probes contain circuitry that is potentially susceptible to damage from electrostatic discharges. Although the probes are input protected against static discharge, when you approach the Omni it is good practice to dissipate any static charges accumulated on your body by touching the chassis before touching the probe pins. Likewise, much digital equipment is static sensitive. You should touch the chassis of any equipment you are testing before making probe connections to it or touching the internal circuitry. Take these precautions after plugging in the power cord to establish a ground connection.

When you are using the Omni as a CP/M computer, the probes need not be connected and you can use it at an ordinary desk or table.

5.2 SETTING UP THE KEYBOARD

Place the Omni flat on your work surface. The keyboard also serves as the front cover, and is held on by clamps on the right and left sides. Unfasten the clamps and remove the keyboard. Connect the telephone-type coil cord between the connector on the keyboard (on the rear edge) and the connector on the main unit (on the rear panel, near the top). If there are two telephone-type connectors on the main unit, use the one labeled "KEYBOARD."

You can lift the main unit and lower the stand on the underside so that the screen is tilted up and easily visible.

The Omni is shipped with cardboard packing cards in the floppy disk drives to protect the read/write heads. Open the doors of both drives and remove the cards. Save the cards for whenever you may want to ship the unit in the future.

Disk drive doors open at turn-on and turn-off!

Turning the machine on or off with a disk in the drive and the door closed may result in scrambling the data on the disk. Opening the drive door moves the head away from the disk, preventing power transients from affecting the data on the disk. It is all right to have disks in the drives at turn-on and turn-off as long as the doors are open.

If you anticipate a possible power interruption - due to a lightning storm or electricians working on the power mains in your building, for example - open the drive doors even while using the Omni, closing them only when file reads or writes are required. (This won't work with a program which uses overlays, such as Wordstar, since the program automatically performs disk accesses when you may not expect it.)

If you do scramble the data on a diskette, then you will have to use your backup diskette to make a new working copy. And if you don't have a backup...

5.3 POWER ON

The power switch is the large rocker switch on the rear panel. Turn it on now. The drives will start whirring and you will soon see:

* Omni *

Please insert your diskette into Drive A

Insert whichever diskette you are going to use in Drive A. To use the Omni as a logic analyzer, use the Logic Analyzer Operation Disk.

It is all right to put a disk in the Omni while the drive is whirring and the red light on the drive is on. (This is not true for all computers). To put the disk in the right way, hold it with the label up. Do not fold the floppy disk, touch the magnetic recording surface, or put it near magnetic materials.

5.4 MASTER MENU

When you close the door of the drive, the computer will load the operating system and display the Master Menu - see Exhibit 5-1. A new feature that makes the system very easy to use, the Master Menu automatically provides information about each menu choice.

Earlier Omni models (1984 and prior) do not have the Master Menu feature and use the standard CP/M user interface. (The standard interface may be reached from the Master Menu by pressing <ESC>). The last section of this chapter, section 5.8, covers the differences of the older units.

The Master Menu groups the files on a disk into categories. Initially, information about the categories is displayed. When you move the cursor-bar to a category using the cursor keys, the individual items in that category are listed along with information about them. When you indicate an individual item, more detailed information about it appears.

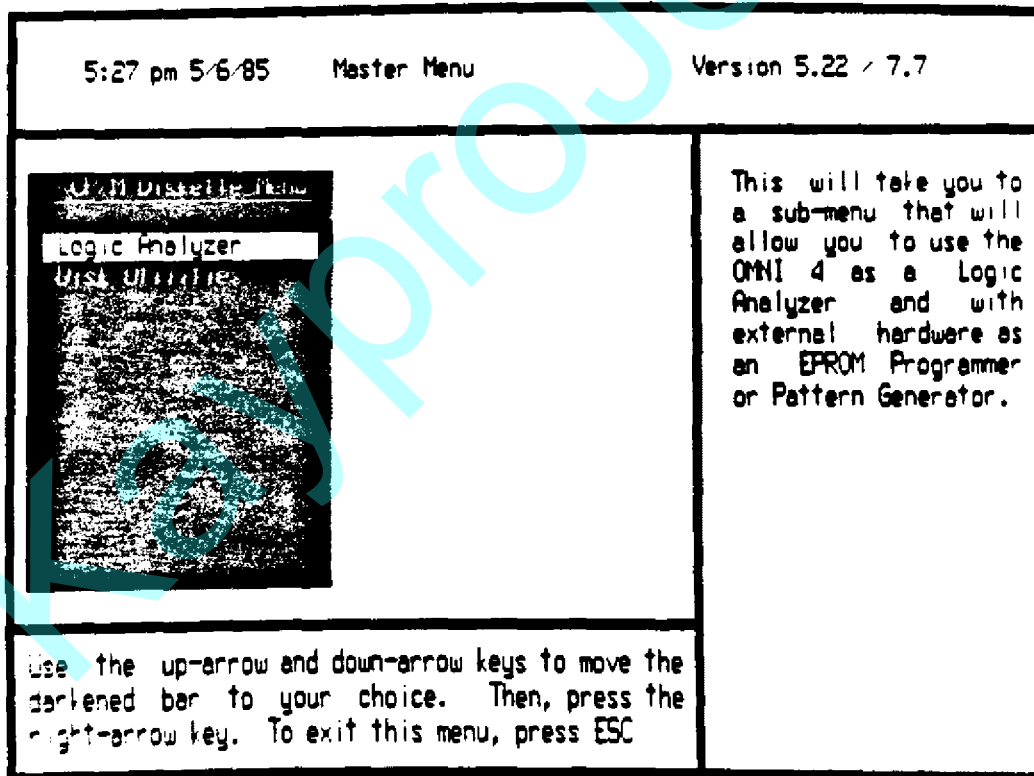


Exhibit 5-1. Master Menu.

For the Logic Analyzer Disk, the two categories are:

Logic Analyzer
Disk Utilities

Use the up-arrow and down-arrow keys to move the dark bar area over "Logic Analyzer". Then press the right-arrow key. The list of individual functions available will be displayed in the middle column:

Logic Analyzer
EPROM Programmer
Pattern Generator

To activate one of the functions, simply move the bar over it and press <RETURN>. If you activate "Logic Analyzer", for example, the Omni will load and begin running the logic analyzer program.

5.5 USE A WORKING DISK

Two copies of the logic analyzer software are provided, a Master Disk and an Operating Disk. Put the Master in a safe place and use the Operating Disk as your working disk. Only masters are provided for the other software. Make working copies and set aside the masters before using the other software.

See the Specifications Section for the type of disks required.

5.6 COPYING DISKS

All Omni models, both those equipped with the Master Menu and earlier units, have convenient disk copy programs.

From the Master Menu select "Disk Utilities" and then "Copy a Disk." A menu will appear with four choices - C, B, O, and E. But before making a selection, remove the disk in Drive A and insert the disk you wish to copy. This is the source disk.

Put a blank disk, the destination disk, in Drive B; this will become the copy. (You can use a disk here that is not blank, but it will be reformatted as part of this copy method and anything on it previously will be erased.) After the prompt line, choose C:

Please enter selection. Press C, B, O, or E ==>C

Note: your input is underlined here to distinguish it from data displayed by the computer.

The program will then display some more information, after which you type <RETURN>:

...press the RETURN key to start the copy operation. You may return to the main menu by pressing any other key.<RETURN>

Note: here "<RETURN>" means "press the RETURN key," not type the characters "< R E T U R N >".

The program will display the track numbers as it makes the copy, and will report errors if there are any. If there are errors, start the copy operation over; if it does not work the second time, the destination disk is probably bad - use another.

After the files are copied, the program will ask if you want a special command line executed at boot-up. You do not, so merely type <RETURN> to accept the default case.

The program then returns to its main menu. Choose "E" to exit.

...Press C, O, B, or E ==>E

The last step in making a copy is to label it. Do not write on the label after it is on the disk with a pencil or ballpoint pen; you can use a felt tip pen, which requires very little pressure. We suggest that you include on the label the version of CP/M, the files on the disk, and at the bottom of the label your initials and the date.

5.7 OPERATING THE LOGIC ANALYZER

To use the Omni as a logic analyzer, put the operating disk (labeled "Omni Logic Analyzer Operating Disk") in Drive A. The Logic Analyzer Disk must be in Drive A for the built-in Help Pages to be accessible.

Press the Reset button. When the Master Menu appears, select "Logic Analyzer" as described above. The computer will load the logic analyzer program and run a series of self-tests. See Exhibit 5-2. If you have the probes plugged in and connected to nothing, the tests will be valid and the screen will display several messages reporting the results.

These tests check out the logic analyzer hardware only, from the ends of the probes to the sample collection circuitry. The tests will be passed only if the probe cables are connected to the Omni and the probe leads are "open" - not connected to anything. If the probes are not installed, or if they are connected to a circuit, a failed test will be indicated on the screen.

If one or more tests fail, the Omni will display failure messages and stop. You may override the stop-on-fail by pressing <SPACE>; the logic analyzer will then go on to the next step, which is the Trigger Condition Setup Menu.

The following chapters describe use of the Omni Logic Analyzer for digital measurements.

You can exit the logic analyzer program and return to computer mode by using CONTROL-C whenever the input prompt (cursor) is in the lower left corner of the screen.

OMNI IV Rev 87/38/84
Inverting Probes

CLOCK CIRCUITRY TEST
TRIGGER CONTROL TEST
PROBE TEST
DATA RAM LOW LEVEL TEST
DATA RAM HIGH LEVEL TEST
GLITCH RAM LOW LEVEL TEST
GLITCH RAM HIGH LEVEL TEST

Test complete with no errors

Exhibit 5-2. Self-test display.

5.8 EARLIER MODELS

Earlier models of the Omni (1984 and prior) use the standard CP/M disk directory user interface. The logic analyzer functions are all the same.

The earlier models use the program COPY.COM to copy disks. Put a disk containing the CP/M operating system in Drive A and boot up (which loads the operating system into the computer) by pressing the Reset switch. The Reset switch is the red button on the rear panel of the Omni II and 4. Don't flip the rocker switch and turn off the computer by mistake.

If the disk with CP/M does not also have COPY.COM on it, put a disk containing COPY.COM in Drive A before the next step. You can use the DIR command to see if the disk has COPY.COM on it.

After the A0> prompt, type "COPY<RETURN>" to run the copy program:

A0>COPY<RETURN>

From this point, the program runs as described above.

To use the Omni as a logic analyzer, reset it and put the Logic Analyzer Operating Disk in Drive A. To see a directory listing of the files on the disk, after the "AO>" prompt type "DIR<RETURN>".

The directory will show at least six files. LA.COM and LA.LAO are the logic analyzer program. LA.LAH contains the Omni's on-line Help information. DATA-1-.LAD, DATA-2-.LAD, and DATA-S-.LAS contain sample data for this start-up exercise.

When the "AO>" prompt appears again after the directory listing, type "LA<RETURN>". The Omni will load and begin running the logic analyzer program, starting with the self-test as described above.

Rev. D

6. BASIC OPERATION

The Omni's basic operation may be summarized as follows:

1) Once connected to a circuit and told to "Go collect data", the Omni begins to collect data into the 16 channels (or optionally 32 channels) of its Sample Memory from the circuit under test. The data is "clocked in" - a new data sample of 16 bits, one bit for each probe data line, is gathered with each clock pulse. The clock pulses are either derived from the circuit under test (External Clock), or generated by the Omni (Internal Clock). The Omni continually collects data and records it in Sample Memory, overwriting old data as it cycles through memory, until a trigger event occurs.

2) The recognition of a trigger word (chosen by the operator) in the data stream causes the Omni to start a counter that defines the number of additional samples to be collected. Data collection continues so that the defined number of samples after the trigger word are captured for observation. The number of samples from the trigger word to the end of the trace is called the Trigger Point. The default value is 500, which gives a trace with the trigger word in the center of the 1000-word Sample Memory.

3) The Omni then displays on the screen the data in its Sample Memory. The display shows a history of the digital activity in the circuit, both before and after the trigger word. The trigger word is at the center of the screen.

Thus a logic analyzer, like an oscilloscope, collects data corresponding to voltage versus time and displays it as "traces".

Two features make the logic analyzer a very powerful tool:

1) It can collect data on many lines at once; in this case, on 16 (or optionally 32) lines. Observing the bit stream on a single line at one time, as with an oscilloscope, is of little value since the bit pattern is meaningful only in comparison to the simultaneous bit patterns on other lines.

2) The logic analyzer displays data prior to the trigger event, as well as after. The oscilloscope only starts the trace at or after the trigger event. When a digital circuit goes awry, the cause is usually found in what happened beforehand, not afterwards.

On the other hand, a logic analyzer has two limitations compared to an oscilloscope. It records voltages as only "high" or "low" (binary 1 or 0), ignoring the details of waveform shape. Also, it records the logic level only at the active clock edge. This second limitation is overcome to some extent by glitch capture capability, which alerts the user to the presence of multiple transitions between clock edges. The Omni's specifications guarantee detection of glitches as narrow as 10 nanoseconds, and it will typically record glitches as brief as 6 or 7

nanoseconds, depending on the polarity.

The time scale resolution is limited to the minimum clock period that the logic analyzer can handle. The Omni will accept a clock frequency of up to 20 MHz, yielding 50 nanoseconds resolution. If finer resolution is required, there is a Trigger Output on the rear of the analyzer that provides an output pulse when the trigger word occurs. This signal can be used to trigger a 200 MHz oscilloscope, giving far greater resolution when a recurring trigger word is available.

After the data around the trigger event has been collected, it can be displayed in a variety of formats for convenient study and interpretation. The Omni's display formats are:

Waveform Display - format similar to timing diagrams in digital data books.

Edge Waveform - same format as Waveform, however in regions where the data is not active, the data is compressed so that only regions of the Memory where the data is changing are displayed.

Dump - format similar to computer memory dumps where logic levels are represented as numbers and grouped as hexadecimal, binary, octal, signed or unsigned decimal digits.

Matrix - format where the numbers of occurrences of logic level combinations are shown in a matrix format.

Instruction Disassembly - format where logic level patterns are displayed as microprocessor instruction mnemonics.

Histogram - provides information on the amount of time a computer spends executing different parts of a program, based on data collected from the address bus.

Signature Analysis - calculation, display, and comparison of signatures for up to fourteen circuit nodes at one time.

Scrolling through the data is facilitated by commands for direct cursor positioning, cursor arrow keys, and a Locate command which finds desired logic patterns. The ability to individually label each channel aids in the readability of the display. With this feature, the names of the circuit points to which the probes are connected can be displayed directly on the screen.

Analysis is aided by displays which show time or number of samples since the trigger event; commands which allow the calculation of sample number and time intervals; and the correlation of the collected data with data previously collected and saved on a disk file. The ability to produce a printed version of any screen display allows several sets of data to be collected for analysis at a later time or for use in consultation with others familiar with the circuit under test. This same feature can be used to produce a record of properly operating circuits for later reference.

Several features have been incorporated in the Omni to make it user-friendly. Most data entry is via menus, with the cursor placed at the position of current activity. Immediate feedback is given after each keystroke, and prompts are given at appropriate times to inform you of the type and range of inputs desired. The inputs are queued so that you can type as fast as you desire without concern that keystrokes will be lost (this applies to the logic analyzer program only; queuing features vary for other programs when using the Omni as a computer.) The cursor position is highlighted for easy location. At any time, you can access a list of commands or information on any command. The format of each command, applications, and examples of its use are provided by the on-screen Help Pages. This feature virtually eliminates the need to refer to this or other manuals once you are familiar with the Omni's basic operation.

Rev. D

7. CONNECTING THE PROBES

7.1 INTRODUCTION

The Omni has 22 input lines that connect via probes to points in the circuit you are testing. The lines are:

- 16 Data lines
- 1 Clock
- 1 Clock Qualifier
- 1 Trigger
- 1 Trigger Qualifier
- 2 Grounds

The 16 data lines collect the digital data which will be stored as samples in the Sample Memory, then later displayed.

The Clock line allows data collection synchronously with an external clock, such as a microprocessor system clock. You may not wish to sample on every pulse of the system clock, but only on clock pulses synchronous with some other event. The Clock Qualifier allows you to use this second event to qualify the data collection.

Usually, you will be triggering on a certain combination of bits on the data lines, called the trigger word. However, on occasion you may wish to trigger on some external event. The Trigger line allows this. You may also wish to qualify the trigger with some other event, and the Trigger Qualifier line allows this. The Trigger Qualifier signal may also be used as a seventeenth bit for word recognition.

7.2 INPUT PODS

The 22 lines connect to the Omni via two pods, 11 lines to each pod:

<u>Pin</u>	<u>Signal</u> <u>Left Pod</u>	<u>Signal</u> <u>Right Pod</u>	<u>Suggested</u> <u>Lead Color</u>
1	Clock	Clock Qualifier	Yellow/White
2	D0	D8	Black
3	D1	D9	Brown
4	D2	DA	Red
5	D3	DB	Orange
6	D4	DC	Yellow
7	D5	DD	Green
8	D6	DE	Blue
9	D7	DF	Violet
10	Trigger	Trigger Qualifier	Red/White
11	Ground	Ground	Green/White

The two pods connect via 36-inch, special high-flex ribbon cables to connectors on the front panel of the Omni. See Exhibit 7-1. While

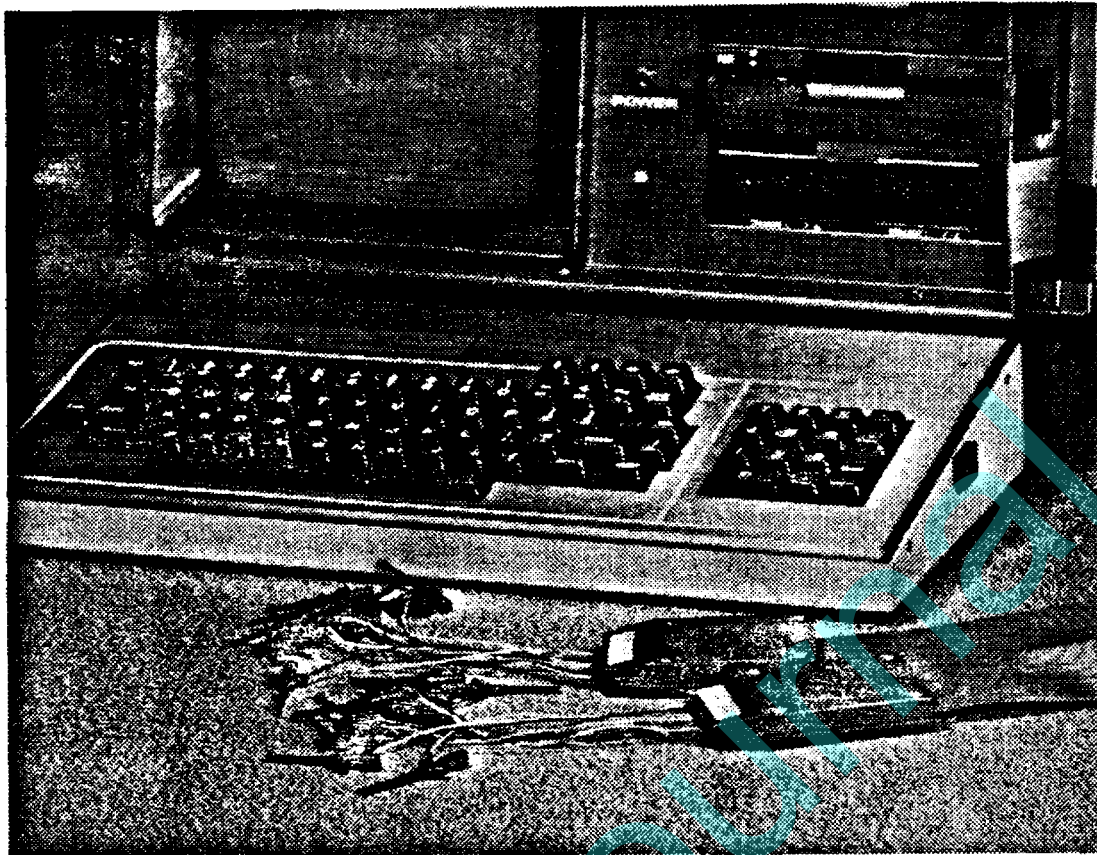


Exhibit 7-1. Omni input leads and pods. The input connectors are inside the opening in the front panel below the disk drives; the cables were not plugged in when this photograph was taken.

facing the machine, "Left" and "Right" refer to the ribbon cable connectors on the main unit; the "left pod" is whichever pod is plugged into the left connector. The pods themselves are identical.

The right pod carries the eight high order channels, DF-D8. The left pod carries the low eight channels, D7 through D0. Of these, the lowest four channels, D3 through D0, contain enhanced circuitry which will capture glitches. If you wish to use glitch detection, connect the low four channels of the left pod to the points you wish to test. Otherwise, no special orientation is needed when connecting the probe assemblies.

Each input pin at the buffer pod accepts a 6-inch test lead terminated in a pushbutton "grabber" clip. The "grabber" is small enough to attach to the pins of standard integrated circuits, which have 0.1 inch pin spacing. The grabbers hang on quite securely.

The Omni is normally supplied with 22 grabber clips and leads. The clips are of special construction for secure connection to small, closely spaced conductors such as integrated circuit pins. They are designed to rotate so that the pods and leads may be moved about without the clip twisting loose from the pin. The lead wires are made with over 100 tiny strands of copper for maximum flexibility and resistance to breakage. The leads have a special locking connector that holds the lead securely to the pod, yet releases easily when desired.

Eleven of the clip-leads are ganged together, while the other eleven are separate. The leads are color-coded to make channel identification easier; we recommend that the various color leads be plugged into the buffer pods in the order listed in the table above.

7.3 TTL OR CMOS

The pods contain buffers that minimize the load on the circuit under test while allowing the Omni to be several feet from the test point. The input impedance of the pods is 1 megohm. Buffer pods are currently available for two logic families, TTL and CMOS. The appropriate one should be selected for the type of circuit under test. A TTL level buffer pod is normally supplied with the unit. For measurements on CMOS circuits, the CMOS buffer pod is preferred. It is possible to utilize one TTL buffer pod and one CMOS buffer pod if analysis is to be performed on circuits which contain both CMOS and TTL. Where one pod is to be used for both types of logic, select the TTL pod. Note the difference in threshold levels between the TTL and CMOS pods in the characteristics listed below.

TTL Buffer Pod Characteristics:

- o logic level transition to low level at 0.8 volts
- o logic level transition to high level at 2 volts
- o minimum detectable pulse 10 nanoseconds
- o maximum voltage limits $-0.5V$, $+5.5V$
- o input impedance 1 megohm

CMOS Buffer Pod Characteristics

- o logic level transition to low level at 1.0 volts
- o logic level transition to high level at 3.5 volts
- o minimum detectable pulse 10 nanoseconds
- o maximum voltage limits $-0.5V$, $+5.5V$
- o input impedance 1 megohm

7.4 PROBE POLARITY

The probe circuitry inverts the polarity of the signals. As part of the power-on self-test, the Logic Analyzer program checks whether inverting probes are connected or not and configures the software appropriately. Thus if the probes are connected when you load the Logic Analyzer program, the polarity will be correct. If you do not connect the probes until after self-test, you will also need to call up the Options Menu (O Command) and change Item 5, Probe Type, from Non-inverting to Inverting. Merely accessing the item toggles the entry from one state to the other.

7.5 CHANGING TEST SETUPS

It is often convenient to utilize multiple sets of test clips when changing from one test setup to another. Using this technique, it is easy to go back to an earlier setup by swapping the test clips at the pod rather than having to reconnect each of the eight test clips. This feature is further enhanced by utilizing the file input/output features

of the analyzer to save and restore channel identification labels. Refer to the File Operations section for details.

Each pod has its own ground line. The ground line should always be connected to a convenient ground position on the circuit under test. It is usually a good idea, especially when glitches or high frequency signals are being monitored, to place the ground clip near the probe clips. This will produce the most accurate representation of the signals as seen in the circuit under test.

NOTE:

Failure to connect the ground clip can cause misleading information to be collected by the analyzer.

If, after connection to the test circuit, the probes should be placed in the wrong pod, or the pods exchanged in their connections to the front of the Omni, no damage will be done. However, any interpretation of the collected data will likely be meaningless until the inversion is detected and corrected.

7.6 CLOCK AND TRIGGER OUTPUTS

Clock Output and Trigger Output signals are available at the rear of the Omni at connector pins mounted directly on the logic analyzer data collection board. They are high speed, TTL level signals suitable for triggering an oscilloscope or other digital processing equipment. The outputs are isolated from the other circuitry through dedicated 74LS04 buffers. Thus loading on these outputs will not affect logic analyzer operation.

Exhibit 7-2 shows the connector pinout for the Clock Output and Trigger Output. Each connector has two pins 0.025-inch square, spaced 0.1-inch apart. The top pin carries the signal and the lower pin is ground.

The falling edge of the Clock Output signal is synchronous with the sampling window for the Omni's data input lines. It is valid for both Internal Clock and External Clock operation. The Clock Output's active edge is the falling (negative going) edge, regardless of the Clock Polarity chosen for External Clock operation.

The Trigger Output signal is active high. It is valid for all modes of trigger operation - Internal or External Trigger, Latched or Unlatched, qualified by the Trigger Qualify or not. The Trigger Output signal is derived from the trigger signal that actually initiates completion of data collection in the Omni.

The Trigger Output signal may be used to trigger an oscilloscope for examination of waveform shapes. For example, it may be desirable to observe operation of power circuitry controlled by a single-chip microcomputer system. Use the Omni to trigger on the digital

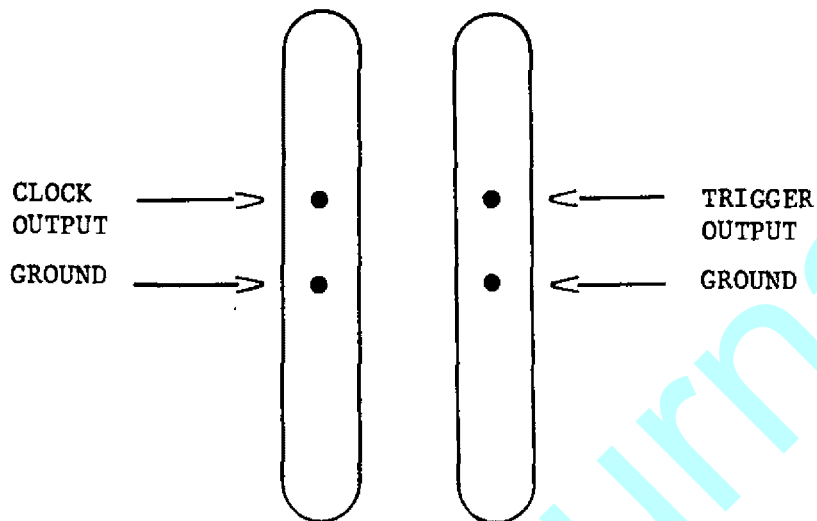


Exhibit 7-2. Clock Output and Trigger Output connector pinouts. The two connectors are accessible through vertical slots in the rear panel of the Omni.

conditions, and the oscilloscope to examine the power signals. In such a case, it may be desirable to force the microprocessor into a loop to give a reasonable repetition rate for the scope trace.

The Trigger Output may also be used to trigger a wide bandwidth oscilloscope for high resolution study of digital signals. For example, with a 200 MHz oscilloscope, waveform details as fine as 1.5 nanoseconds can be observed. By providing the necessary trigger signal to allow the oscilloscope to display the digital events of interest, the Omni makes possible ultra-high-resolution measurements beyond the normal capability of either a logic analyzer or oscilloscope alone.

With the Omni operating in the Internal Clock mode, the Clock Output may be used as a convenient signal source where an accurate, stable digital clock signal is required. For example, the Clock Output may be used as the clock source to test clock-driven digital circuits such as counters, shift registers, and state sequencers. Since the Omni's data collection is synchronized to the clock, collecting state data to track the operation of these circuits is very easy.

8. MENUS AND COMMANDS

8.1 INTRODUCTION

The Omni needs three kinds of input from you to operate:

Trigger and sampling conditions for collecting the data - trigger word, clock pulse polarity (for external clock), and so on. This information is entered on the Trigger Condition Setup Menu (Trigger Menu for short). The initial entries on this menu default to the most commonly used values.

Go Command - causes the Omni to start collecting a new data sample and looking for a trigger condition.

Display selection - set up the Omni to display the collected data. The default display is the Waveform Display, which shows the signals as a timing diagram. Also available are the Dump Display, which lists the data as hexadecimal, binary, octal or decimal numbers, and several other special purpose displays.

Two methods are used to control the Omni: Menus and Commands. Menus are used to set up the event recognition method (either trigger word in the input data stream or External Trigger signal), Sample Rate, and other control parameters. Commands control the format in which the collected data is displayed.

8.2 MENUS

The menus are called up by single letter commands. For example, "O" will call up the Options Menu. The single letter suffices; it is not necessary to press <RETURN>.

The menus and the letter commands that call them up are:

<u>Command</u>	<u>Menu called up</u>
C	Correlation Menu
F	File Operations Menu
H	Histogram Menu and Display
L	Locate Pattern Menu
O	Options Menu
P	Pattern Generator
S	Signature Analysis Menu
T	Trigger Menu
Z	Complex Trigger

Each menu shows the present values of the parameters it controls. On power-up, the most commonly used parameter values are installed as defaults. See Exhibit 10-1 for an example of the Trigger Menu, the most frequently used menu.

To enter a new parameter in a menu item, type the item number to move the prompt-cursor to the item, then enter the desired parameter value. If the item has more than one data entry field, press <RETURN> to move to the next field. For example, Item 3 on the Trigger Menu has both binary and hexadecimal entry fields; press <RETURN> to move from the binary field to the hexadecimal field.

Press <SPACE> to leave an item and return the prompt-cursor to the lower left corner of the screen.

8.3 COMMANDS

Commands control the collection and display of data. Commands are made up of a command letter and one or two optional parameters. The commands that collect or display data are shown below. Optional parameters are shown in square brackets, "[]".

<u>Command</u>	<u>Effect</u>
D[x]	Numeric dump from sample x
E[x]	Edge display from sample x
G	Go collect data
I[x]	Instruction disassembly from sample x
M[x[,y]]	Matrix display from sample x to y
W[x[,y]]	Waveform display from sample x to y
=	Load trigger word and collect data

Additional commands that perform various useful functions are:

<u>Command</u>	<u>Effect</u>
?[C/D,...]	Help Pages for Commands C, D,...
N#xyz...	Name Channel number # with xyz...
CTRL-P[x[,y]]	Print copy of sample x to y
X[x[,y]]	Calculate time between cursor, x, or y

When you enter the first letter of a command sequence, the format for the rest of the command appears immediately on the prompt line. Do not put a space after the command letter; the space is inserted automatically. When you enter two numeric parameters, use a space to separate them. All commands except "G" and "=" must be ended with <RETURN>.

As an example, consider the command:

W5<RETURN>

"W" calls up a Waveform Display of the most recently collected data. The parameter "5" causes the display to start from Sample 5, the fifth sample after the trigger event.

If you make an error in the middle of a command sequence, type "</RETURN>" to abort the command, then re-enter the command correctly.

Commands are accepted when the prompt-cursor appears in the lower left corner of the screen,

Both lower and upper case characters are accepted; lower case is treated internally as uppercase. The "W5" command could have been typed as "w5" with the same result. The slash character "/" is accepted as "?", a comma is accepted as "<", and a period is accepted as ">". Thus one-finger typists do not need to use the shift key.

8.4 REPRESENTATION OF DIGITAL SIGNALS BY NUMBERS

As the name "digital logic" implies, electronic signals may be used to represent numbers, and vice-versa. The basic form of representation is binary, where, for example, an eight-digit binary number such as "1001 0111" is used to represent the signals on eight electrical lines. Each digit in the binary number is a "0" or a "1", representing a high voltage level (HI) or low voltage level (LO) on the corresponding line.

Let us represent the form of the binary number like this:

abcd efgh

Here "a" represents the first bit, "b" the second, and so on. The number may be evaluated by multiplying the bits by powers of 2 and summing:

$$N = a*2^7 + b*2^6 + . . . + h*2^0$$

Thus "a" is the high-order bit, "b" is the next bit, and so on to "h", which is the low-order bit. Extending the correspondance between the eight bits and the eight signal lines, we may apply mathematical terminology to the signal lines. The line corresponding to the high-order (leftmost) bit is the high-order line, and the line corresponding to the low-order (rightmost) bit is the low-order line.

For the Omni, we call the signal lines channels. They are labeled according to the powers of two in the binary number. Thus eight of the channels are called Channel 7, Channel 6, and so on to Channel 0. We may also call Channel 7 the high-order channel (in this group of eight), and Channel 0 the low-order channel.

Binary numbers are difficult for people to deal with. When expressing digital signals as numbers, it much more convenient to use a number base such as decimal (base 10), hexadecimal (base 16), or octal (base 8). Note, however, that the correspondance between the digits of the numbers and the signals is lost when decimal is used. "173" may represent the signals on Channels 7 through 0 very nicely, but the "7" does not correspond to the signal on any one channel or group of channels.

Hexadecimal representation is often preferred because each hex digit does correspond exactly to the signals on four channels; a hex digit is equal to four bits. A signal on the Omni's 16 channels may be represented by four hex digits, e.g., "9AC5". In this context, "9" corresponds to the signal(s) on Channels F-C, "A" to Channels B-9, and

so on. To interpret this in terms of signal levels, translate it to binary. Thus "9" is equal to "1001" in binary, which means a HI level on Channel F, LO on Channel E, LO on Channel D, and HI on Channel C.

8.4 FORMAT FOR ENTERING NUMBERS

Most entered data is numeric and can be specified in a variety of formats. All numbers are assumed to be in hexadecimal format, unless indicated otherwise by a base suffix. To enter a number in another base, such as decimal, append one of the following base specifiers:

<u>Suffix</u>	<u>Base</u>	<u>Valid Digits</u>
B	binary	0 and 1
D	decimal	0,1,...,9
H	hexadecimal	0,1,2,...,9,A,B,C,D,E,F (default radix)
O	octal	0,1,2,...,7
U	unsigned decimal	0,1,...,9

Typical input values are:

<u>Example</u>	<u>Meaning</u>
1234	decimal 1234
1234D	decimal 1234
-1234	decimal negative 1234
47H	hexadecimal 47 (i.e. decimal 71)
ABCDH	hexadecimal ABCD (i.e. decimal 43,981)
1011B	binary 1011 (i.e. decimal 11)
17O	octal 17 (i.e. decimal 15)

The term "radix" is sometimes used as a synonym for "base."

The "sample number" for a given sample means the position of the sample compared to the trigger event, which normally corresponds to Sample 0. For example, in the "W5" command referred to earlier, the number "5" indicated 5 samples after the trigger event. Samples before the trigger event are indicated by a negative sample number such as "W-5". Note that if a nonzero value is specified for the Delay on the Trigger Menu, Sample 0 will be delayed with respect to the trigger event by that amount.

If time units are desired rather than sample number, then the number should be suffixed with time units. These units are:

<u>Suffix</u>	<u>Meaning</u>
NS or N	nanoseconds (.000000001 second)
US or U	microseconds (.000001 second)
MS or M	milliseconds (.001 second)
S	seconds

The command:

W5u<RETURN>

will generate a Waveform Display of the collected data with the sample 5 microseconds after the trigger event positioned at the left side of the screen. Numbers are maintained to three significant digits after the decimal point and you are allowed to enter numbers which contain decimal points. The following examples illustrate some valid number representations.

<u>Example</u>	<u>Meaning</u>
500ns	500 nanoseconds after the trigger event
-5500us	5500 microseconds before the trigger event
-5.5ms	same as previous example (i.e. 5.5 milliseconds before)

A number such as "500.75ns" is overly precise since the resolution of the analyzer is limited to the nearest 50 nanoseconds. This number would be accepted as "500ns".

8.5 CURSORS

The Omni uses two cursors, called the prompt-cursor and the highlight-cursor. The prompt-cursor is a blinking block or underline that shows where characters entered from the keyboard will appear on the screen. The highlight-cursor, also called the sample cursor, is a highlighted area of the screen used to mark a certain sample in a display. The highlight-cursor also uses either a vertical line to indicate the marked sample (for the Waveform and Edge Displays) or a "<" character (for the Dump Display).

8.6 DISPLAY CONTROL KEYS

Displays are controlled by the following keys:

<u>Key</u>	<u>Function</u>
>	scroll display one page to right
<	scroll display one page to left
<-	move highlight-cursor one position left
->	move highlight-cursor one position right
↑	scroll display or highlighted item up one position
↓	scroll display or highlighted item down one position
<SPACE>	exit current menu or display

8.7 HELP INFORMATION

A list of all the commands appears on the Reference Card, Appendix B at the end of this manual, and in abbreviated form on a label on the keyboard. The list is also available on-line as two Help Pages; see the next section for further information on the Help Pages.

Rev. D

9. HELP PAGES

Help Pages may be called up as needed. Whenever the command line

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,(sp),^P

appears, a list of the menus and commands may be obtained by typing "?<RETURN>".

This list is the same as that given on the Reference Card at the end of this manual, Appendix B. The first half of the list appears on the screen immediately; to view the second half, press <SPACE>.

More detailed information about any menu or display command may be obtained with a question mark followed by the command letter, for example:

?W<RETURN>

A Help Page will appear that gives details on the format and use of the W Command, which controls the Waveform Display.

The Help Pages are contained in disk files that are presented in response to commands beginning with "?". The Logic Analyzer Disk must be in Drive A for the Help Pages to be accessible.

After viewing a Help Page, press <SPACE> to return to the menu or display you were viewing before.

The menus have additional Help Pages on-line for each menu item. Type "?" followed by the number of the menu item to see a detailed explanation of the item. For example, on the Correlation Menu, "?5" gives a detailed explanation of Item 5, Starting Point Skew Allowance. Exhibit 9-1 shows the Correlation Menu and the corresponding Help Page for Item 5. After reading the explanation, press <SPACE> to go back to the menu.

When the first letter of a command is keyed in, abbreviated Help information for the command is automatically displayed. The information appears as a prompt line that gives the format for the command or a description of its effect.

1) File to correlate with: INTERNAL
2) Channel mask: FEDCBA9876543210
1111111111111111
3) First sample included: 25
4) Number of samples: 100
5) Starting skew allowance: 25
6) Skew alignment samples: 1
7) Sampling tolerance: 5
8) Channel (bit) tolerance: 0
9) Repeat data collection until: A
-> A) (not active)
B) Samples correlate with reference
C) Samples do not correlate with reference

Index 1-8, G to start, P, ?, or (space)

(a)

5) STARTING POINT SKEW ALLOWANCE

The starting point given in Item 3 specifies a sample number in the Sample Memory and implies the same in Reference Memory. Due to sampling differences, these two starting points may not be exactly at the same sample number. To account for this, Item 5 allows you to skew the Reference Memory starting point some given value. The value entered is the maximum number of samples on either side of the implied starting point that should be allowed. For example, a value of 10 for the starting point and 4 for the skew would mean that the Reference Memory starting point could be anywhere from 6 to 14.

Hit key to continue

(b)

Exhibit 9-1. Correlation Menu (a) and the Help Page for Item 5 (b).

10. TRIGGER CONDITION SETUP MENU

10.1 INTRODUCTION

The trigger word and other trigger conditions are entered in the Trigger Condition Setup Menu, Exhibit 10-1, usually called the Trigger Menu for short. It is the first page that appears after self-test and the command lists when you load the logic analyzer program, LA. You may also call it up with the T Command.

For the simplest form of triggering, enter the desired trigger word in Item 3, Trigger Event. The trigger word is expressed both in binary form, which allows "don't care" bits (each denoted by an "X"), and in hexadecimal form at the right of the binary field.

The menu format makes entering the trigger word very easy. Type "3" to move the prompt-cursor to Item 3. The prompt-cursor will begin blinking in the first column (labeled "Channel F" at the top) to show that the Omni is ready to accept an entry in that column. You can move the cursor to another channel either by using the left and right arrow keys, or by entering the channel designator "F" through "2" ("1" and "0" are not available for moving the cursor since they are used as entry symbols.) Key "5", for example, will move the cursor directly to Channel 5.

Keying in a "1", "0", or "X" for a given channel sets the trigger level for that channel to high, low, or "don't care", respectively. The cursor then moves to the next channel.

The Omni also allows triggering on logic functions (AND, OR, and NOT) of the bits in the collected samples. In order to facilitate this, the sixteen channels are divided into four groups of four bits each. The four groups are labeled "z", "y", "x", and "w". In addition, Channels 3 through 0 have glitch triggering capability; the glitches are considered Group g. Item E, Recognition Function, defines the logic function of the five groups which initiates triggering. Type "E" to move the prompt-cursor to Item E, then key in the number of the desired logic function.

After setting the trigger conditions, type "G" for "Go and Collect Data." The Omni will collect data, stop after the trigger condition is satisfied, and display the new data in the current display format.

When you finish viewing a data display and are ready to reset the trigger conditions to collect another display, press <SPACE> to bring up the Trigger Menu again. You can also reach the Trigger Menu by typing "T".

If you wish to display less than all 16 channels, or wish to display glitches on the lower four channels, Items 1 and 2 allow you to set up those conditions.

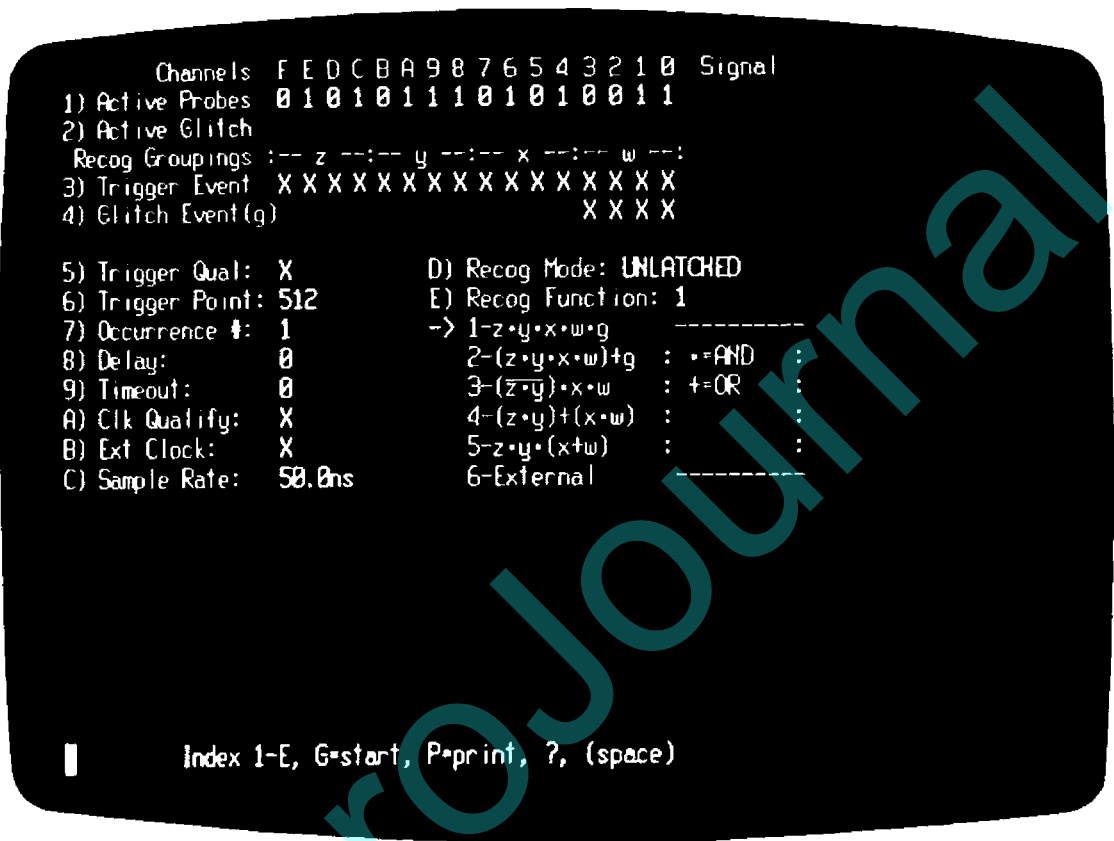


Exhibit 10-1. Trigger Menu as it appears on the screen.

10.2 SAMPLE CLOCK

The Omni uses a clock signal, called the sample clock, as its cue to sample the logic level on the sixteen input lines. A sixteen bit word, one bit for each channel, is collected on the active edge of the sample clock. (The active edge may be either the rising or the falling edge.) The sample clock may either be a signal generated by the Omni itself (Internal Clock), or a signal derived from the equipment under test (External Clock).

Use of the Internal Clock is often referred to as asynchronous sampling (not synchronous with signals in the equipment being tested), or "timing analyzer mode." To activate this mode, enter a Sample Rate in Item C. The default mode is Internal Clock mode with a Sample Rate of 50 nanoseconds (50 nanoseconds between samples). Using the Internal Clock, the clock edge used (rising or falling) is not meaningful to the measurement and is not specified.

Use of the External Clock is often referred to as synchronous sampling, or "state analyzer mode." To activate this mode, enter the desired clock edge, "1" or "0" (rising or falling), in Item B; Item C will be updated to show "External Clock" automatically.

There is often some confusion between clocking and triggering when using a logic analyzer for the first time. It takes 1000 clock edges to fill the trace memory with 1000 samples. It takes only one trigger event to stop data collection and give a display. We recommend that you always use Internal Clock and manual trigger for your first measurement in any testing. That will show you the signals on the input lines, no matter what they are. We also recommend that you go through the Quick Start procedure (Appendix A) the first time you attempt to use the Omni.

10.3 GLITCHES

A "glitch" is a narrow pulse, usually created as a spurious by-product accompanying state changes in a logic system. Address decoders and other multi-gate circuits often produce glitches when some parts of the circuit respond slower than others, yielding illegal states that last for less than a clock cycle.

In synchronous (clocked) logic, glitches are usually harmless since they occur between active clock edges, and hence are ignored. Sometimes, however, they cause trouble, and when they do, the Omni may be used to detect them and isolate the source.

Basic logic analyzer circuitry, which collects data only at the active clock edge, will not normally detect glitches. The Omni contains latches that follow the incoming data stream; if two or more level transitions occur within one clock period, that is considered a glitch. Detection of the glitch is recorded in a special glitch memory. When glitches are present and glitch display is activated, glitches appear on the Waveform Display as narrow pulses.

Channels 3 through 0 have the ability to capture glitches. Item 4, Glitch Event, controls triggering on glitches. Enter a "1" to activate glitch triggering on a given channel, or an "X" to disable. The glitch polarity is not significant; when a "1" is entered, the Omni will trigger on glitches of either polarity in that channel. Entering a "0" has the same effect as entering a "1".

If glitch triggering is activated for more than one channel, appearance of a glitch on any one activated channel will satisfy glitch recognition.

10.4 = COMMAND

The = Command is a combination command that allows you to both change the trigger word and initiate triggering at the same time. To use it, line up the sample cursor, in the Waveform or other data display, on the word you wish to use as the new trigger word. Then type "=" to load the word marked by the cursor into Item 3, Trigger Event, and start data collection. When you use the "=", the trigger event will

be the value displayed at the trigger position. Any channel that is not displayed (i.e., not active) will take on an "X" (don't care) value in the trigger word.

10.5 TRIGGER POINT AND DELAY

A trace of approximately 1000 samples is collected during each data collection run (approximately 500 samples when using the 32 channel adapter). Normally, the trigger event will correspond to a point approximately in the center of the trace, so that there are 500 samples before the trigger event and 500 samples after the trigger event.

The sample corresponding to the trigger event is normally labeled Sample 0. The other samples are numbered relative to the trigger event; thus Sample 5 is the fifth sample after the trigger event, Sample -10 is the tenth sample before, and so on.

Sometimes it is desirable to observe samples that are more than 500 sample clocks before or after the trigger event. Two menu parameters, the Trigger Point, Item 6, and the Delay, Item 8, make it possible to do this. Exhibit 10-2 shows how these two parameters skew the collected data in time relative to the trigger event.

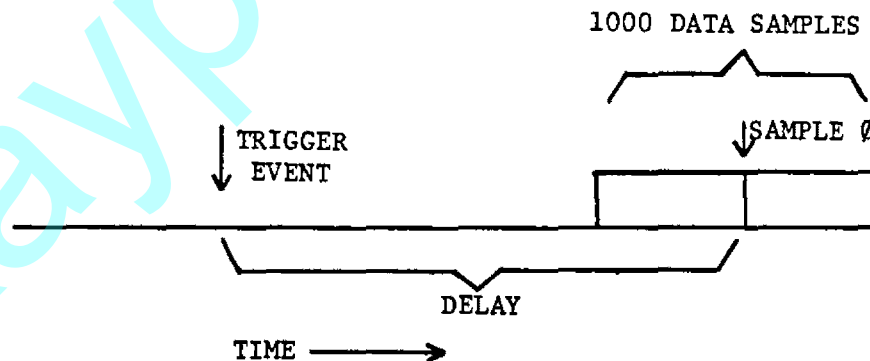


Exhibit 10-2. Relationship between the trigger event, Delay, Trigger Point, and Sample 0. The ability to specify independently the Delay and Trigger Point makes it possible to view data before, after, or long after the trigger event. Note that when the Delay is 0 (the default case), Sample 0 is simultaneous with the trigger event.

The Trigger Point defines the number of samples that the trace extends past Sample 0 (which normally corresponds to the trigger event). For example, a value of 96 will cause 96 samples to be saved after the trigger, and thus approximately 900 before; the trace will extend from (approximately) Sample -900 to Sample 96. The default value for the Trigger Point is 512, which puts Sample 0 in the middle of the collected data.

By setting the Trigger Point to 992, 992 samples after the trigger event may be observed. If data is to be collected at some longer time period after the trigger event, then a Delay parameter (Item 8) can be specified. This will skew the collected data some specified time after the trigger. The value of the Delay corresponds to the time difference (expressed as a certain number of sample clocks or as an absolute time value) between the trigger event and Sample 0. Thus when a non-zero Delay is present, Sample 0 does not correspond to the trigger event. Only positive delay values are allowed. (The capability of accepting negative delay values has not been implemented, as this would require that the instrument be capable of predicting the future.)

10.6 AN EXAMPLE

The availability of many different trigger parameters vastly increases the Omni's power to isolate and capture a particular event. For example, assume that you have an eight bit microprocessor system that is supposed to be moving a zero out of the accumulator at a certain instruction in its program, but sometimes a non-zero number appears and disrupts system operation.

To capture this event, you could connect Channels 7 through 0 to the lowest eight address lines, and Channels F through 8 to the data bus. For the Trigger Event, enter the lowest eight bits of the address of the critical instruction in Channels 7 - 0, and zeros in Channels F - 8. Use Section 3 of the Recognition Function (Item E) to achieve triggering when Channels 7 - 0 equal the Trigger Event and Channels F - 8 do not equal the Trigger Event. With these conditions, whenever the critical instruction moves a non-zero number out to the accumulator and onto the data bus, the Omni will trigger on that event and display both address and data bus information before and after.

10.7 MENU ITEMS

Detailed explanations of the individual menu items follow. To enter a parameter in a menu item, first press the key corresponding to the number of the item, e.g. press "1" to move the prompt-cursor to Item 1. After the change has been made, press <SPACE> to leave the item and return the prompt-cursor to its home position at the lower left.

Item 1) Active Probes

This item has two functions. One, it shows the instantaneous logic levels on the input probe lines for the channels that will be included in the data displays. Two, it shows which channels will be included in the data displays, and provides a way of selecting the channels which will be displayed.

A high or low logic level on each input probe line is indicated by a "1" or a "0". The level display is updated several times a second and a varying logic level will cause the display to flicker between "0" and "1". Channels not included in the displays will have a blank space in the corresponding bit position in this item.

To activate a given channel for display, first press "1" to move the cursor to this item. Then keys "F", "E", "D", ... "0" will activate the corresponding channel. Or, use the "<->" and "<->" cursor keys to move the cursor to the desired channel, and press any other key except "X". To deactivate a channel, press the "X" key. The keys auto-repeat.

Note that when you move the cursor to a channel, the channel label appears to the right under "Signal".

Exit this item with <SPACE>.

This item affects only the display format; it has no effect on data collection (data is always collected on all channels) or triggering.

Item 2) Active Glitch

This item selects the channels for which glitches will be displayed on the Waveform and Edge Displays. Channels with a "#" symbol will display glitches, others will not. Glitch capability is limited to Channels 3 through 0. To activate a given channel, first press "2" to move the cursor to Item 2; then key "3" or "2" will move the cursor to the corresponding channel and activate it. Or, use the "<->" and "<->" cursor keys to move to the desired channel, then press any other key except "X" to activate it. To deactivate the channel, press the "X" key. Press <SPACE> to leave this item.

This specification affects only the display format; it has no effect on data collection (data is always collected on all channels) or triggering. Glitch display can be activated only for channels also active in Item 1.

Item 3) Trigger Event

When the Omni encounters the word entered in this item in the data stream, it will trigger, stop data collection after the specified number of additional samples, and display the collected data. To set the trigger condition for a given channel, move the cursor to that channel. Keys "F", "E", . . . "2" will move the cursor to the corresponding channel, or the "<->" and "<->" cursor keys may be used. For each channel, enter a "1" to choose a high logic level as the recognition condition, or a "0" to choose a low level. Enter an "X" to choose a "don't care" condition. Item 3 defaults to all "don't cares" on power-up.

After entry, the trigger word also appears in hexadecimal notation at the right of Item 3. "Don't care" bits are valued at 0 in the translation to hexadecimal. To enter the trigger word directly in hexadecimal, press <RETURN> to move the cursor into this field from the

binary field. Direct hexadecimal entry does not allow "don't cares."

Press <SPACE> to leave this item and return the prompt-cursor to the lower left.

Item 4) Glitch Event (g)

Any of the four channels in Group w can enter into the recognition event by entering a "1" when the cursor is positioned at the desired channel. No glitch is an "X". The cursor positioning commands are the same as for Item 3. Unlike the Trigger Event, however, the glitch channels operate on an OR logic condition. If any one (or more) of the selected glitch channel detects a glitch, recognition occurs.

Item 5) Trigger Qual.

Trigger qualification can be specified by entering a "0" or "1" in this item. "X" disables trigger qualification. "1" indicates that the probe Trigger Qualify line must be at a high logic level before an event can be recognized; when the input line is at a low level, all data input to the event recognizer is ignored. "0" indicates the opposite condition, that is, the event can only be recognized when the Trigger Qualify input is at a low level. Essentially, the Trigger Qualify acts as a 17th channel (or as a 33rd channel when the 32 channel option is installed) for trigger event recognition.

To use Trigger Qualification, Line T on Probe Pod B (right pod) must be connected to the trigger qualifying signal.

Item 6) Trigger Point

A 1000-sample trace is collected about the trigger event during each data collection run. The number of samples that the trace extends past the trigger event (which normally corresponds to Sample 0) is specified with this item. A value of 90 will cause 90 samples to be saved after the trigger, and thus approximately 900 before. A value of 500, the default condition, puts the trigger event approximately in the middle of the collected data.

Item 7) Occurrence

This specifies the number of times the trigger event must occur before recognition takes place. An occurrence is counted each time the trigger pattern goes from a state where the signal does not match the trigger pattern, to one that does match the trigger pattern. The length of time for a match or no-match condition has no bearing on the occurrence counting. Selection of 1 to 15 occurrences is supported.

Item 8) Delay

Usually data will be collected immediately around the trigger event. However, if data is to be collected at some time period after the trigger event, then a delay can be specified. This will skew the collected data some specified time after the trigger. The delay can be specified as a certain number of sample clocks or as an absolute time

value. Absolute time delay is selected by using suffixes to indicate time units: "ns" or "n" for nanoseconds; "us" or "u" for microseconds; "ms" or "m" for milliseconds; and "s" for seconds. No suffix implies that the delay parameter represents number of samples, rather than time units. Depending on the sample rate, the delay can range from 16 microseconds to 34 seconds. Only positive delay values are accepted. The delay and timeout resources are shared, so that when either is selected, the other is disabled.

Item 9) Timeout

This function provides a means of detecting when a certain pattern (which normally occurs repetitively) is absent for a specified time or longer. The pattern is entered in Item 3, Trigger Event, and the time limit, called the Timeout period, is specified in Item 9. If a Timeout period goes by during which the (normally repetitive) event has not occurred, then a trigger will be generated and data collected.

For example, consider the case of a microprocessor-based controller which is required to poll several input devices periodically. If the controller fails to respond to a service demand within a certain time, a fault condition occurs. This can be caused by the processor getting "tied up" spending too much time on one task. To solve the problem, it is necessary to identify which task is tying up the processor when a fault - failure to poll the input device - occurs. Set up the Omni to collect microprocessor addresses, which will identify program tasks. Set up the triggering so that Item 3, the Trigger Event, corresponds to polling of the critical input device. For the Timeout period, enter a time value equal to the normal interval between the polls of the input device. Then when the input device is not polled on schedule, the Omni will execute a trigger sequence, that is, halt data collection and display the data. The addresses of the offending time-consuming task will be captured in the data.

The Timeout period depends on the Sample Rate and can vary from 16 microseconds to 34 seconds. It can be specified either as a certain number of sample clocks or in time units. Enter time units in the same way as described above for Delay, Item 8. The Delay and Timeout resources are shared, so that when either is selected, the other is disabled.

Item A) Clk Qualify

Sampling normally occurs on every cycle of the signal (external or internal) being used as the sample clock. If there are periods when data collection should not be performed, the Clock Qualify line can be used to limit the collection to only the desired periods. For example, it may be desired to collect only data bytes sent to a particular I/O port. This may be achieved by using the I/O write strobe as the External Clock, and using the decoded port select signal in the port circuitry for Clock Qualify.

Entry of a "1" in this item causes data to be collected only when the Clock Qualify line is high. A "0" enables data collection only when the Clock Qualify line is low. If no qualification is desired, enter an

"X" to specify the "don't care" condition.

To use Clock Qualification, Line C on Probe Pod B (right pod) must be connected to the clock qualifying signal. In the example above, that would be the decoded port select signal.

Item B) Ext Clock

When synchronous data collection is to be performed, the External Clock selection should be used and the desired sampling edge specified. If the sample is to be saved on the low to high transition of the clock, enter a "1" (positive going) edge. A negative going edge is selected with a "0" entry. To deselect the External Clock, either enter "X" in this item or specify an Internal Clock Sample Rate in Item C.

To collect data with an External Clock, Line C on Probe Pod A (left pod) must be connected to the signal in the equipment under test that is to be used as the clock signal.

Clock rates up to 20 MHz (50 nanoseconds) are supported.

Item C) Sample Rate

When the Internal Clock is used, a Sample Rate must be chosen. The Sample Rate can be varied from 50 nanoseconds (20 MHz) to 32 milliseconds (30 Hz). For high speed data collection, rates of 50ns, 100ns, 200ns, and 500ns are available. If a rate that is not available is selected, then the next faster available rate will be used. Slower rates can be selected in one microsecond intervals up to 32.766 milliseconds. To specify the sample rate, enter the desired rate followed by a time unit suffix, "n", "u", "m", "ns", "us", "ms", or "s".

Item D) Recog Mode

The Recognition Mode may be Latched or Unlatched. That is, trigger recognition can be performed on data as it passes through the recognizer, or the data can be latched by the sample clock prior to recognition. The Unlatched mode is appropriate when high speed signals of potentially short duration are being detected. The Latched mode should be used when monitoring a data bus type circuit, where data is considered valid only during the clock edges. Selecting this item toggles (changes) the Recognition Mode from Unlatched to Latched, and vice-versa.

Item E) Recog Function

The sixteen data channels and four glitch channels are organized into five groups labeled "z", "y", "x", "w", and "g". These groups may be combined via this item to allow triggering on various logical combinations of data and glitch. For example, Function 1, "z.y.x.w.g", requires that the 16 data lines match the Trigger Event specified in Item 3, and that a glitch appear on one of the channels specified in the Glitch Event, Item 4.

If no Glitch Event (Item 4) is specified, Function 1 will be satisfied when only the Trigger Event (Item 3) is satisfied.

Function 2, "(z.y.x.w)+g", requires only that the Trigger Event or the Glitch Event be satisfied; not both.

Function 3 is " $\overline{(z.y)}$.x.w". Here the overbar symbol means logical negation, that is, " \overline{z} " means "not z". Since "g" does not appear, Function 3 applies only to the sixteen data lines. It is satisfied when, and only when, all three of the following conditions are true: Channels F through C (Group z) do not match the data event; Channels B through 8 do not match the data event; and Channels 7 through 0 (Groups x and w) do match the data event. "Not match" for a group means any one (or more) bits within that group failing to match.

Function 4, "(z.y)+(x.w)", also applies only to the sixteen data lines. It is satisfied when either Channels F-8 (z and y) or Channels 7-0 (x and w) match the data event.

Function 5, "z.y.(x+w)", is satisfied when Channels F-8 (z and y) match the data event, and either Channels 7-4 (x) or Channels 3-0 (w) match the data event.

If Function 6, External Trigger, is selected, then you must also specify the edge of the trigger pulse on which triggering shall occur. Enter "1" for a leading (rising) edge or "0" for a trailing (falling) edge.

To use an External Trigger, Line T on Probe Pod A (left pod) must be connected to the signal in the equipment under test that is to be used as the trigger signal.

10.8 HELP PAGE

When you are viewing the Trigger Menu, you can access Help Pages for Items 1, 2, etc. by typing "?1", "?2", etc. Press <SPACE> after viewing a Help Page to return to the Trigger Menu itself. Help information for the Trigger Menu as a whole may be accessed by typing "?T" when the prompt-cursor appears at the lower left corner of the screen.

10.9 COMPLEX TRIGGER

The Complex Trigger Function allows triggering on a sequence of trigger words, rather than a single trigger word. This capability is also called sequential triggering or multilevel triggering by some logic analyzer manufacturers.

Type "Z" to bring up the Complex Trigger Menu, which controls this function. Exhibit 10-3 shows an example of the menu.



Exhibit 10-3. Complex Trigger Menu.

Calling up the menu enables the Complex Trigger Function. When it is enabled, the trigger pattern is governed by the entries on this menu rather than by Item 3 on the Trigger Menu.

The successive trigger words are entered in Items 2 through 8 of the Complex Trigger Menu. The trigger words must occur in the order listed for triggering to occur. That is, each trigger word must have appeared in the data stream and been recognized before the Omni is ready to recognize the next word. The Omni initially watches for the first word. Once that has been recognized, it watches for the second word and so on. After the last word occurs and is recognized, the Omni completes the data collection and displays the data in the usual way.

There is a delay following recognition of a word in the trigger sequence, called the Setup Delay, until the Omni is ready to recognize the next word. Occurrences of the next word in the data stream before the Setup Delay has expired will be ignored. The Setup Delay has a minimum value of 100 microseconds. Greater time values may be entered in the menu.

The menu also includes a Trigger Mask (Item 1) to limit recognition to a subset of the total sixteen channels.

Accessing Item 9 toggles the Complex Trigger Function between enabled or disabled status; when it is disabled, normal triggering as defined on the Trigger Menu governs the trigger method. The Complex Trigger Function is disabled at power-up.

10.10 EXAMPLE OF COMPLEX TRIGGERING

Many computer software bugs can be localized by collecting the addresses of instructions as they are executed. Studying the flow of program control will reveal which part of the program is at fault.

However, programs often use nested subroutines, or subroutines called from several places in the main program, to perform a complex series of steps. In such cases, there are many "execution paths" that the program may take. Often a troublesome problem is associated with only one execution path. A subroutine may perform correctly sometimes but misbehave other times, depending on where it was called from in the main program. To locate the bug, you need to focus data collection "by path."

The Complex Trigger Function allows you to do exactly that. Enter as trigger words the calling addresses of the successive subroutines in the path you wish to study. The Omni will collect data around the last trigger word, which becomes Sample 0 (typically) in the displayed trace. The sample data will reveal the system behavior that results from that particular path.

10.11 COMPLEX TRIGGER MENU ITEMS

Item 1) Trigger Mask

Not all probe lines need be included in the trigger words. A "1" in a given bit position means that the corresponding bit is considered by the recognition circuits. An "X" means the bit is ignored. The Trigger Mask word is also automatically displayed to the right in hexadecimal notation, where each "X" is assumed to have a value of 0.

Items 2) Trigger Word and Setup Delay

Enter the first trigger word following the "2)". If you wish to specify a setup delay value, use the right-arrow cursor key to move the cursor to the Setup Delay field. Merely press <RETURN> to get the default delay of 100.0 microseconds.

Items 3) through 8)

Enter additional trigger words and (if desired) setup delay values in these items.

Item 9) Complex Recognizer Enabled/Disabled

Accessing this item toggles the Complex Trigger Function between enabled and disabled status. The disabled condition allows you to return to single word triggering (that is, Item 3 on the Trigger Menu

again determines the trigger word) without disturbing the list of words in Items 2 through 8.

10.12 COMPLEX TRIGGER HELP PAGE

To display information for the Complex Trigger function, type "?Z" when the prompt-cursor appears at the lower left corner of the screen. To display information for the individual menu items when viewing the menu, type "?1", "?2", and so on. After viewing the information, press <SPACE> to return to the menu itself.

Kaypro Journal

Rev. D

11. OPTIONS MENU

11.1 INTRODUCTION

The Options Menu (Exhibit 11-1) controls various aspects of the data displays: output number base, sample or time units on the Waveform and Edge Displays, display Sample or Reference Memory, enable modem, probe type (inverting or non-inverting), and disassembly status lines available or not (for the Instruction Disassembly function).

To call up the Options Menu, type "O<RETURN>".

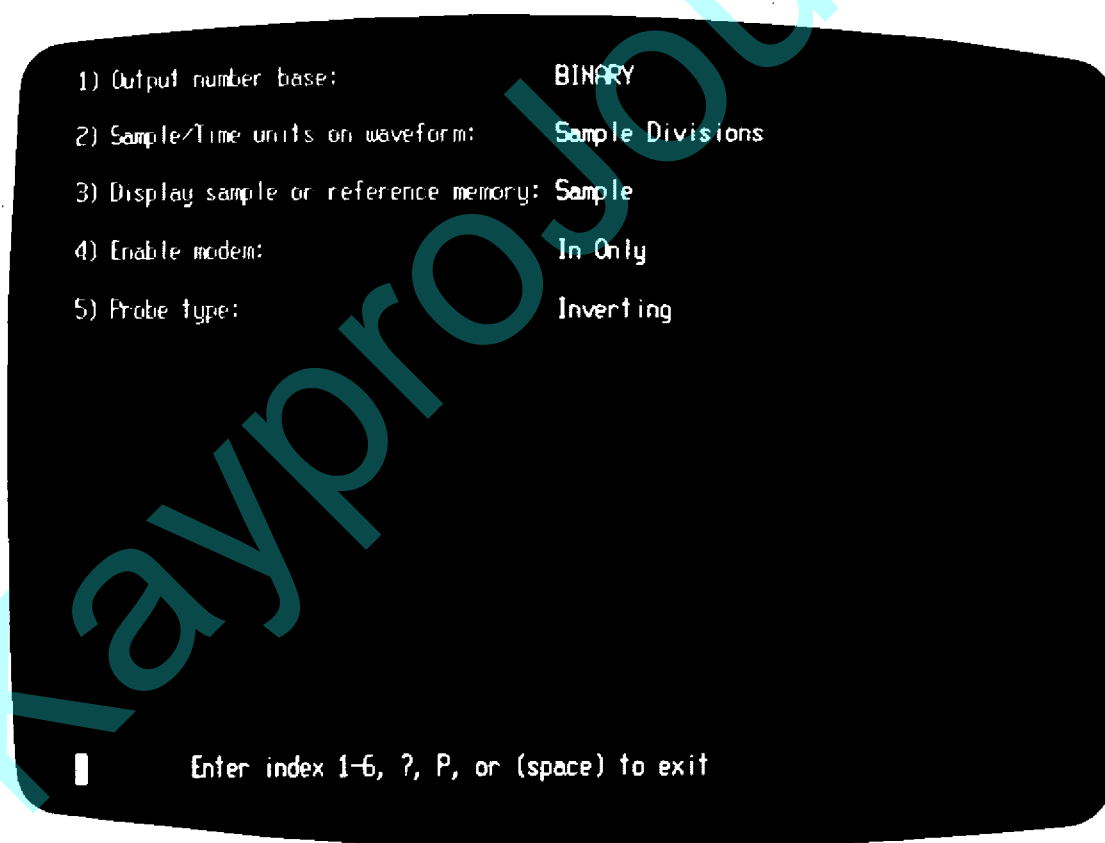


Exhibit 11-1. Options Menu as it appears on the screen.

11.2 MENU ITEMS

To enter a new parameter in one of the menu items, type the item number in order to move the prompt-cursor to the desired item. Following are explanations of the individual menu items:

Item 1) Output number base:

The default output number base is hexadecimal. The menus and displays that show the data in alphanumeric form (Dump, Matrix, and Trigger Setup) use the number base specified in this item.

In hexadecimal notation, the 16 channels are organized into groups of four, and the value contained in each group (each four bits) is displayed as a single hexadecimal digit. The number base can be changed to octal (groups of 3 channels), binary (each digit represents one channel), or one of two decimal representations. The signed decimal grouping treats the Channel F value as the sign bit of a twos complement number. The unsigned decimal format allows only positive values.

After moving the cursor to this item by typing 1, enter one of: octal, B for binary, D for decimal, H for hexadecimal, O for octal, or U for unsigned decimal.

Item 2) Sample/Time units on waveform:

The Waveform and Edge Displays contain a graticule scale which indicates the position of each sample displayed relative to the trigger event. This scale can be labeled either with number of samples before and after the trigger point, or with time units before and after the trigger point. Selecting Item 2 toggles the scale labeling between these two cases. When time units are selected, the values will be displayed in an engineering format to three significant digits. Units of nanoseconds (ns), microseconds (us), or milliseconds (ms) are used.

Item 3) Display Sample or Reference Memory:

When data is collected, it is automatically stored in Sample Memory and displayed in the current display mode. It is also possible to load previously collected data into Reference Memory, and then display the Reference Memory. This facility is useful for making comparisons between two sets of collected data, such as when the correlation function is used.

There are two ways of loading data into Reference Memory. It may be transferred there from Sample Memory, or it may be retrieved from a file previously saved on disk. Sample to Reference transfer is performed via the File Menu. File to Reference transfer can be done from the Correlation Menu or File Menu.

When Reference Memory is selected, all subsequent displays will show it until Sample Memory is again selected or a new data collection is made with the G or "=" Commands. Selecting Item 3 toggles between Sample Memory and Reference Memory.

Item 4) Enable modem:

The Omni 4's internal modem is controlled by this item. Accessing Item 4 toggles the modem status between enabled and disabled. When the Logic Analyzer Program is first loaded, the modem is enabled for input (that is, input from a phone line through the modem will be treated the same as input from the keyboard) and disabled for output (output is sent to the screen, not the modem line).

"Enable" (first access of Item 4) enables the output as well as the input. This allows you to dial up the Omni from a remote location, and control the logic analyzer from the remote location. Transmit "0" to access the Options Menu, then "4" to enable the modem. Once enabled, output goes to the modem rather than the screen. This gives you full control of the Omni over the phone connection. Note that until this full control is established, you will not have any feedback over the phone line - you have to send the "0" and "4" blind.

"Disable" (second access of Item 4) disables both modem input and output, returning full control to the local keyboard and screen. To return to the initial state, it is necessary to exit and then reload the Logic Analyzer Program.

Item 5) Probe type:

The Omni software can accommodate either inverting or non-inverting probes. Accessing this item toggles a software switch between Inverting and Non-inverting settings. All present OmniLogic probes are of the Inverting type, which is the default case for this item. This function is included to provide flexibility for possible future options. It may presently be used where display of negative logic is desired.

11.3 HELP PAGE

The Help Page for the Options Menu may be accessed with "?0". When viewing this Menu, Help Pages for Items 1, 2, etc., may be accessed with "?1", "?2", and so on. When you finish viewing the Help information, press <SPACE> to return the Options Menu itself.

Rev. D

12. GO AND START DATA COLLECTION

12.1 INTRODUCTION

After the probe leads are connected to your circuit and you have entered the appropriate data collection parameters in the Trigger Menu, type "G" to initiate data collection.

The G Command instructs the analyzer to start collecting data using the sampling characteristics defined on the Trigger Menu. With each active clock edge, one sample is collected from the data input lines and loaded into the Sample Memory. The analyzer collects data until the trigger event specified on the Trigger Menu appears. It collects a defined number of samples after the trigger event, and then data collection stops and the data is displayed.

The number of samples collected after the trigger event is defined by the number specified in Trigger Menu Item 6, Trigger Point. The sample collected at the time of the trigger event is labeled Sample 0 in the data display. Thus in the display, the Trigger Point is the number of samples from Sample 0 to the end of the trace.

If the trigger event does not occur, the analyzer will continue to collect data indefinitely. Likewise, if the sample clock stops after the trigger event but before the number of samples called for in Item 6 has been collected, the analyzer will not complete the trace. In both of these cases, the analyzer appears to be waiting. If triggering does not occur after a reasonable length of time, press any key except <SPACE> to end data collection, initiate a manual trigger, and display the data collected to that point.

Pressing <SPACE> will abort sample collection without a trigger and return to the Trigger Menu. The data in the Sample Memory will not change.

The "=" Command, like the G Command, also initiates data collection. However, before starting data collection, it enters the sample marked by the sample-cursor as the trigger word in Item 3 on the Trigger Menu. See Chapter 10 for more information on the "=" Command.

12.2 DISPLAY FORMATS

<u>Command</u>	<u>Display Mode</u>
W	Waveform Display
E	Edge Display
D	Dump Display - hexadecimal, octal, binary or decimal listing
I	Instruction Disassembly Display
H	Histogram Display
M	Matrix Display

Upon completion of data collection, the Omni will display the data in Sample Memory in one of the above six display modes - whichever one was used last. On first use, the Waveform Display appears. A different display mode may be selected by typing the appropriate command letter, "W", "E", "D", "I", "R", or "M", followed by <RETURN>.

12.3 HELP PAGE

To display the Help Page for the G Command, type "?G".

KayproJournal

Rev. D

13. WAVEFORM DISPLAY

13.1 INTRODUCTION

The Waveform Display gives a simultaneous view of up to 16 channels of digital information that was collected by the Omni. The format is similar to timing diagrams found in digital data books, and is particularly helpful for hardware troubleshooting. It is the default display mode at turn-on. The collected data will be shown in the Waveform Display until another display format is chosen.

13.2 SCREEN CHARACTERISTICS

An example of the Waveform Display is shown in Exhibit 13-1. The display is 80 samples wide. A sample was collected for each cycle of the signal used as the sample clock. Since the maximum clock rate is 20 MHz, the finest resolution that can be obtained with the Waveform Display is 50 nanoseconds between samples. (Waveform details can be viewed to higher resolution by using a wideband oscilloscope and the Trigger Output signal; see Section 7.)

Features of the display are:

Channel labels - at left side of the screen. The default labels are DF, DE, and so on through D0. The additional 16 channels available with the 32 channel option default to AF through A0. The labels shown in Exhibit 13-1 (DATA7, MREQ, etc.) are user-selected labels entered using the N Command.

Waveforms - show the high and low logic levels versus time on the sixteen data lines.

Glitches - shown as narrow pulses if glitch display is enabled and any glitches are present.

Movable highlighted cursor - marks Sample -466 for further attention.

Graticule - beneath the waveforms. Identifies the samples relative to the trigger point, and is calibrated with either sample numbers or time divisions (as specified in the Options Menu, O Command).

Hex codes - in vertical columns beneath the graticule. Represent the hexadecimal equivalents of the data above. "FC52" is marked by the cursor and highlighted by increased brightness.

SM or RM - to the right of the window. Indicate whether the data being displayed is in the Sample Memory or the Reference Memory.

<G or G> - if shown, mean there are glitches to the left or the right of the cursor. <G> indicates glitches to both the right and the left.

ref: - indicates the sample used as a reference by the X Command, that is, the sample from which an interval is measured. The X Command is a utility that calculates the interval, in number of samples and time, between two samples. See Section 16 for further information on the X Command.

cur: - identifies the position of the highlighted sample cursor relative to the trigger event (Sample 0). When the Internal Clock is used, the time interval between the sample marked by the cursor and Sample 0 can be calculated, as it is equal to the number of samples in the interval times the Sample Rate. The Omni calculates the time interval and displays it here.

?_ - at lower left. This is the home position of the prompt-cursor. Commands entered by the user appear here.

Enter: - shows the commands which may be entered next. Press <SPACE> or the "T" key to return to the Trigger Setup Menu.

13.3 COMMAND FORMATS

The Waveform Display is controlled by the W Command by using one of the following command formats:

W Display data as waveforms while centering the sample marked by the highlighted cursor in the previous display. For example, if you wish to move the display 20 samples to the right, move the cursor 20 samples to the left of center and press "W<RETURN>". The display will then move 20 samples to the right.

Wx Display data as waveforms starting from sample x. x is entered in sample number units. If Internal Clock is being used, x may also be entered time division units.

Wx,y Display data as waveforms from sample x to sample y.

WALL Display data as waveforms from first through last sample.

The form Wx will always cause 80 samples (less a few covered up by the channel labels) to be displayed. The form Wx,y will always cause at least 80 samples to be displayed, even if y-x is less than 80.

If y-x is greater than 80, samples from x to y will be "time compressed" to provide a "zoom lens" view of the data that is useful for finding data patterns of interest quickly. However, this feature must be used with care for the following reasons.

With compression, the HI or LO level shown in each column on the screen for a given channel may really be the algebraic sum of several samples. For example, if $y-x$ is equal to 240, then each of the 80 HI or LO levels shown for Channel 0 really represents three samples in the data. If the three samples are all HI, then the screen will show a HI, and fairly represent the data. On the other hand, if the three samples have a mix of logic levels, then the logic level displayed will be based on "majority rule."

The compressed display depicts the data most fairly when there are few transitions in the data. If there are many closely spaced transitions, detail is lost.

13.4 COMMAND EXAMPLES

W16 Display data as waveforms starting at sample 16.

W-500,500 Display "zoom" of data from samples -500 to 500.

W300ns Display data from the sample at 300 nanoseconds.

13.5 DISPLAY CONTROL KEYS

The highlighted cursor or the entire display may be scrolled right or left using these keys:

- < scroll the display horizontally one page to the left with an overlap of 5 samples (75 samples displayed)
- > scroll the display horizontally one page to the right with an overlap of 5 samples (75 samples displayed)
- <- move the highlighted cursor one sample to the left
- > move the highlighted cursor one sample to the right

These four keys auto-repeat; hold the key down for repeated scrolling or cursor movement.

13.6 HELP PAGE

To display the Help Page for the W Command, type "?W<RETURN>".

Rev. D

14. EDGE DISPLAY

14.1 INTRODUCTION

The Edge Mode Display is a compressed version of the Waveform Display. It might also be called the Transition Display, because it displays transitions only. Most repeated occurrences of the same pattern are not displayed, thus showing samples only where the data is changing. If three or more consecutive samples in all the channels to be displayed remain in a steady state, the data will be removed and the display will show a vertical blank where the steady state data was removed.

Exhibit 14-1 is an example of the Edge Display as it appears on the screen.

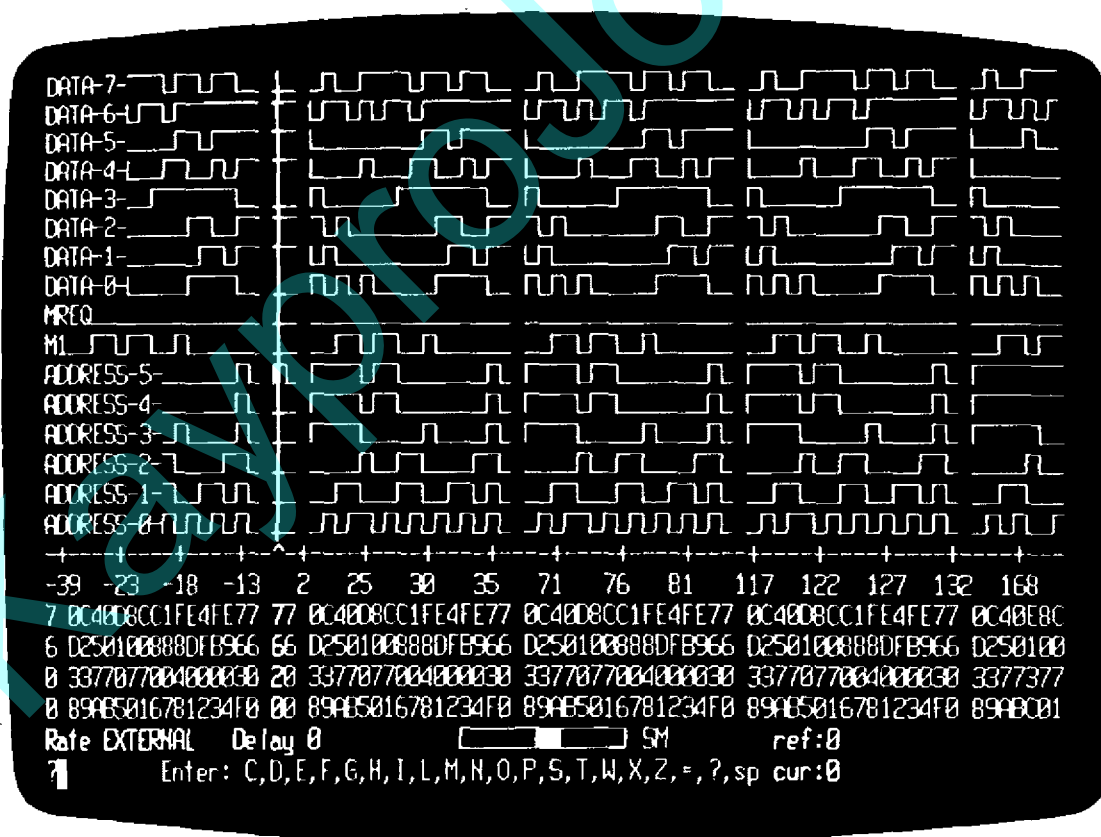


Exhibit 14-1. Edge Display. The E Command causes data in the Sample or Reference Memory to be displayed in this format.

14.2 SCREEN CHARACTERISTICS

Explanations of the data appearing in the Edge Display are given below.

Channel labels - left side of screen; default to the DF, DE ... D1, D0 shown on the Trigger Menu and on the probes at power-on. The labels shown here (DATA-7-, MREQ, etc.) are user-specified labels which were entered with the N Command.

Waveforms - for active channels show the transitions versus time on the displayed data lines. Time periods where no transitions occur (i.e., 3 or more consecutive samples without a change in any of the selected channels) are displayed as a single blank column. The value of the data during the time period represented by the blank column is the same as the data shown in the column to the left of the blank.

Glitches - shown as narrow pulses on the waveforms if glitch display is enabled and any glitches are present.

Highlighted cursor - marks a particular sample. Its location is displayed to the right of "cur:". It is movable with the <- and -> keys.

Graticule - located beneath traces; identifies the samples relative to the trigger point. Calibrated in either sample or time divisions (specify on Options Menu, O Command). Time divisions are dependent on Sample Rate selection.

Hex codes - in vertical columns beneath the graticule; represent the hexadecimal equivalents of the data above. The hex value of the sample marked by the cursor is highlighted by increased brightness.

Rate - indicates either the Sample Rate, when the Internal Clock is being used, or External Clock, when an external source is being used as the sample clock. When Internal Clock is used, the Sample Rate is expressed in time units.

Delay - indicates the Delay (of sample 0 compared to the trigger event), a data collection parameter specified on the Trigger Menu.

Window - to the right of the Delay shows where the 80 samples displayed lie in the total 1000-sample memory.

SM or RM - to the right of the window indicate whether the data being displayed is in the Sample Memory or the Reference Memory.

<G or G> - if shown, mean there are glitches to the left or the right of the cursor. <G> indicates glitches to both the right and the left.

ref: - indicates the sample that the X Command uses as a reference point to measure from. The X Command is a utility that calculates the interval, in number of samples and time, between two samples. See Section 16 for further information on the X Command.

cur: - identifies the position of the highlighted sample cursor relative to the trigger event (Sample 0). When the Internal Clock is used, this part of the display also shows the time interval between the sample marked by the cursor and the trigger event.

?_ - at lower left is the home position of the prompt-cursor. Commands entered by the user appear here.

Enter: - shows the commands which may be entered next. Press <SPACE> or the "T" key to return to the Trigger Setup Menu.

14.3 COMMAND FORMATS

The Edge Display is controlled by the E Command using one of the following command formats:

- E Display data as compressed waveforms while centering the sample marked by the highlighted cursor in the previous display.
- Ex Display data in Edge mode starting from sample x. x is entered in sample number units. If Internal Clock is being used, x may also be entered in time division units.
- Ex,m Display data in Edge mode starting from sample x and including only channels defined by m in the edge transition algorithm.

14.4 COMMAND EXAMPLES

- E16 Display data in Edge mode starting at sample 16.
- E300ns Display data from the sample at 300 nanoseconds.

14.5 DISPLAY CONTROL KEYS

The highlighted cursor or the entire display may be scrolled right or left using these keys:

- < scroll the display horizontally one page to the left
- > scroll the display horizontally one page to the right
- <- move the highlighted cursor one sample to the left
- > move the highlighted cursor one sample to the right

These four keys auto-repeat; hold the key down for repeated scrolling or cursor movement.

14.6 HELP PAGE

To display the Help Page for the E Command, type "?E".

KayproJournal

Rev. D

15. NAME COMMAND

15.1 INTRODUCTION

N, the Name Command, changes the channel names that label the traces in the Waveform Display, Edge Display, and Signature Analysis. The Logic Analyzer initially shows labels DF, DE,...D0 for the standard 16 channels. If the 32 channel option is installed, labels AF, AE,...A0 appear for the additional 16 channels. If signals such as a read pulse, write pulse, and two address lines are being probed, more descriptive names such as READ, WRITE, ADDR0, and ADDR1 make interpreting the data much easier.

New labels installed with the N Command also appear automatically on the Trigger Menu. On the Trigger Menu, the label for whichever channel the cursor is on appears under "Signal" when you are entering new parameters in Items 1 through 4.

15.2 COMMAND FORMAT

Use the N Command with the following format:

N#xyz Name channel # as xyz

= channel identifier F,E,..2,1,0

xyz = any character string not over 15 characters long. Spaces are not allowed in the string; use underscore or hyphen characters instead.

14.3 EXAMPLE

NZMEM-READ Name Channel 2 with the label "MEM-READ". Each Waveform, Edge, and Signature Analysis Display, as well as the Trigger and Search Menus, will then contain this label instead of the default label, "D2".

15.4 HELP PAGE

To display the Help Page for this command, type "?N".

Rev. D

16. INTERVAL CALCULATIONS

16.1 INTRODUCTION

The X Command is a convenience feature that calculates the interval, expressed in time or number of samples, between any two samples. You provide the two end points of the interval, and the Omni calculates the time (if Internal Clock is being used) and number of samples between these points. The end points can be entered as parameters with the command, or the highlighted cursor can be used to mark them.

16.2 COMMAND FORMAT


The X Command can be used in one of these formats:

- X Calculate the number of samples and time between the current highlighted sample and the reference sample. The reference sample is the sample marked with the cursor during the previous use of the X command. If the X Command has not been used since data was last collected, Sample 0 is the reference sample.
- Xm Calculate the number of samples and time between the current highlighted sample and sample m.
- Xm,n Calculate the number of samples and time between samples m and n.


16.3 EXAMPLES

- X 10ns Calculate the number of samples and time between the current highlighted sample and the sample that occurred 10ns after trigger.
- X 10,20 Calculate the number of samples and time between sample number 10 and sample number 20.

These commands must be followed by a <RETURN> when they are entered. Do not type the space between the "X" and the "10"; it appears automatically. Note that when two parameters are specified, a comma is required to separate them.

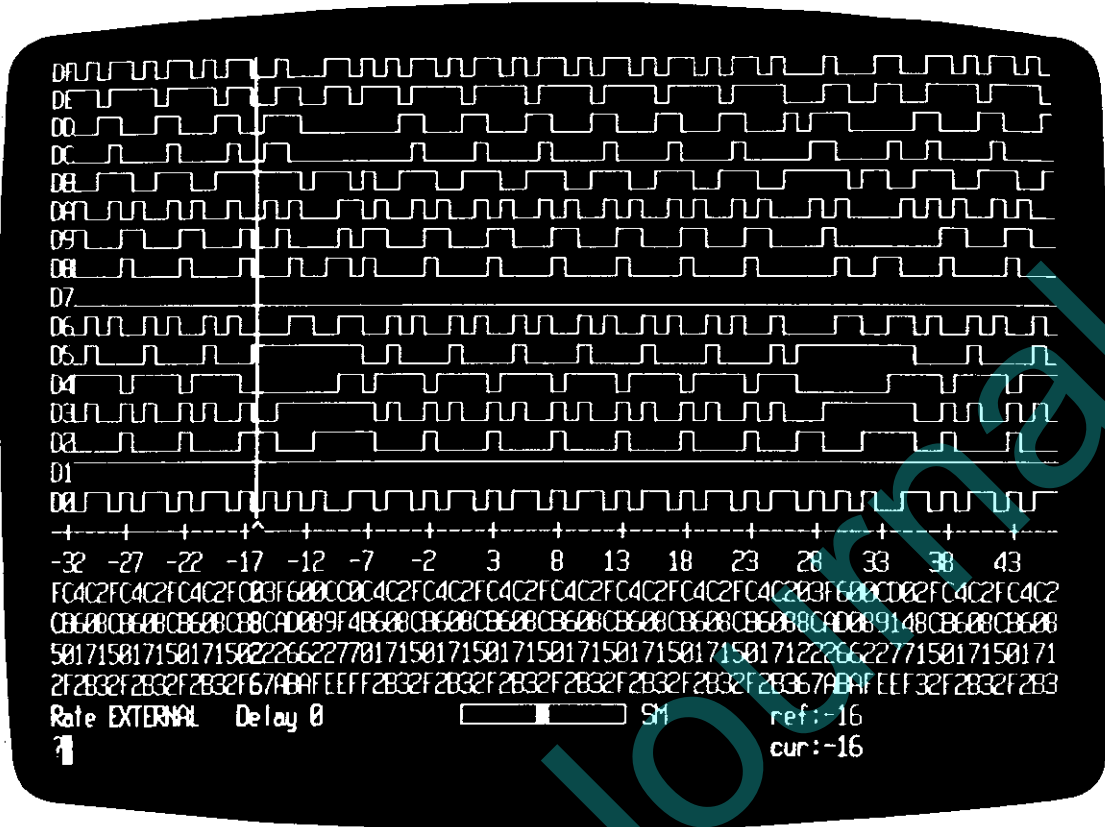

(a)

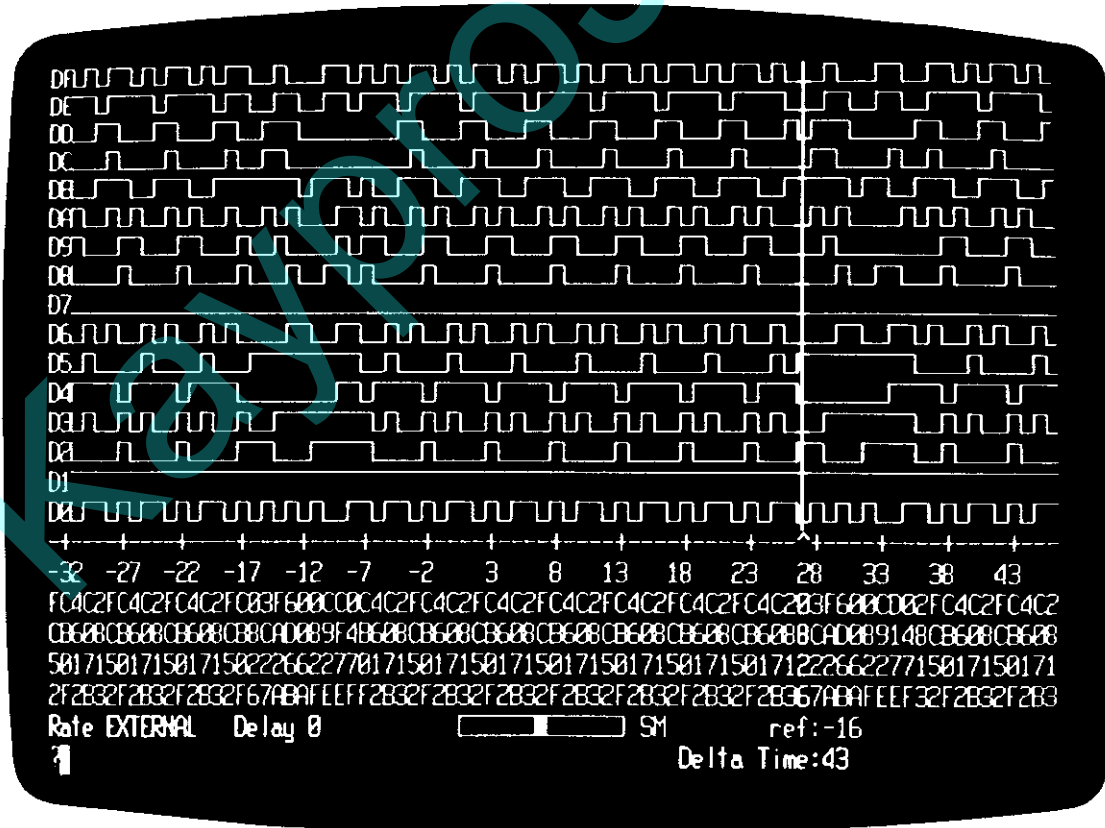

(b)

Exhibit 16-1. Two uses of the Interval function (X Command).

Assume that Internal Clock is being used with a Sample Rate of 5 microseconds. Then the command "X 10,20" will result in this display at the lower right corner of the screen:

Delta Time: 10/50.0us

Sample 10 and sample 20 are 10 samples apart, which is 50.0 microseconds, given 5 microseconds between samples.

It is possible to mix time and sample number units when using the X Command. Assuming the same 5 microsecond Sample Rate, the command

X 10,125us<RETURN>

will give the output "15/75.0us". Sample 10 corresponds to 50us, and 125us corresponds to sample 25.

In another format, assume the display cursor is at sample number 30. The command

X 10<RETURN>

will cause an output of "20/100.0us". Since only one parameter was provided in the command, the cursor position (30) was used as the left point of the interval and the 10 as the right point.

Let us assume that the cursor was positioned on the leading edge of some waveform when the command "X 10" was given, and the cursor has since been moved to the trailing edge of the same waveform at sample number 65. The command

X<RETURN>

will calculate the interval of time between the cursor at last use of the X Command (30), and the current cursor position (65). The output in this case will be "35/155.0us". Using this technique of cursor positioning in conjunction with the X Command, it is very easy to measure time intervals for waveforms, parts of waveforms, or for time between events. For waveform timing, the display will usually be Timing or Edge. With the Dump Display, intervals between events may be calculated by marking them with the cursor and using "X<RETURN>" twice.

Another powerful technique is to use the Locate function to position the cursor on the events of interest, and the X Command to calculate the interval between them. After the first occurrence of the pattern has been found, issue "X<RETURN>" to establish the cursor position as a point of reference. (Ignore the output of this first X Command; we are only interested in establishing a reference for the next use.) Then find the second event with the Locate function. Finally, use "X<RETURN>" again to give you the number of samples and time between the first and second events.

16.4 HELP PAGE

The Help Page for the X Command may be obtained by typing "?X".

Kaypro Journal

Rev. D

17. DUMP DISPLAY

17.1 INTRODUCTION

This display, illustrated in Exhibit 17-1, shows the data in Sample Memory as a listing in hexadecimal, binary, decimal, or octal format. The radix (base) of the display defaults to hexadecimal, but can be changed to binary, decimal, or octal using the Options Menu, O Command.



Exhibit 17-1. Dump Display. The D Command causes data in the Sample or Reference Memory to be displayed in this format. Also, if the data last displayed was in this format, new data collected in response to the G or "=" Command will be displayed in this format. The sample cursor is a "<" symbol next to the highlighted sample in the fifth column.

The same data can be re-displayed in the new base after changing the base; it is not necessary to collect a new sample. This flexibility greatly eases interpretation of the data. For example, control lines are usually best represented in binary, while data lines demand hex or decimal.

Exhibit 17-2 shows the same data as 17-1, but re-displayed in binary notation. The Omni automatically centers the display about whichever sample was marked by the cursor in the previous display.

When the 32 channel option is used, the two banks (of 16 channels each) can be simultaneously displayed with different number bases.

The Dump Display is normally used with External Clock to collect state data.

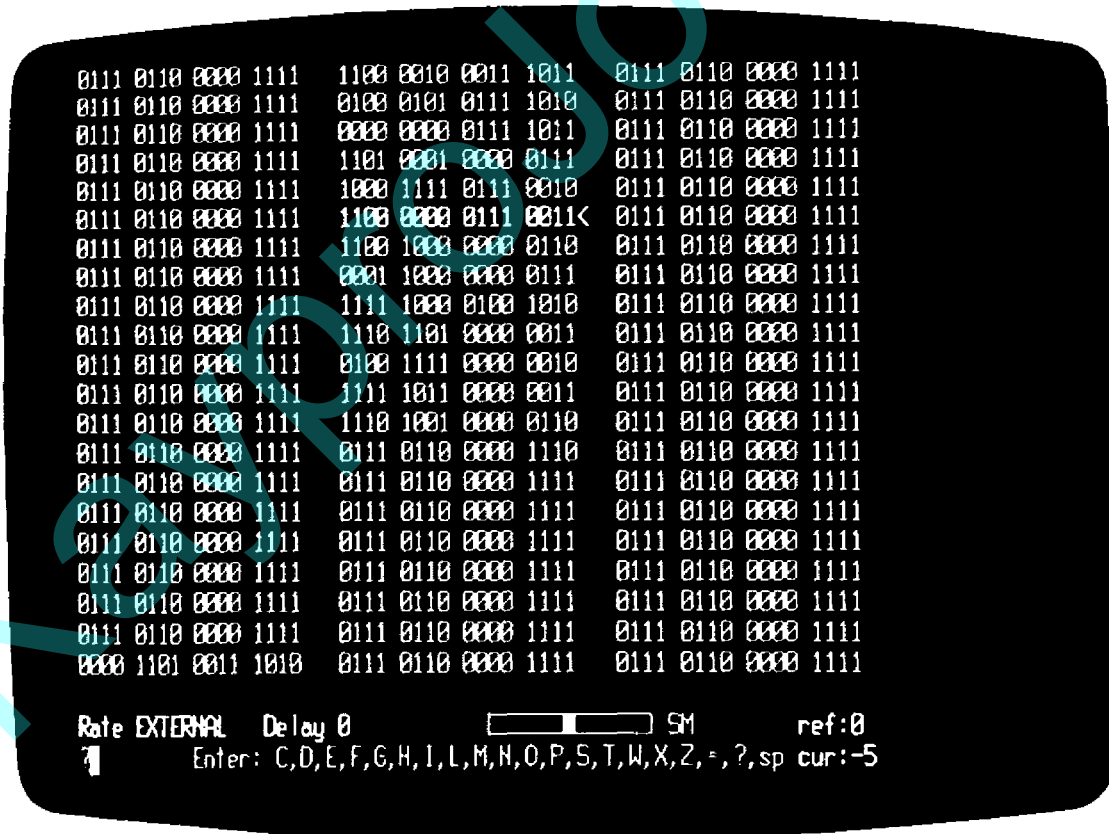


Exhibit 17-2. Dump Display of the same data as in the last exhibit, this time in binary format. The display is centered about the sample marked by the cursor in whichever display appeared previously.

17.2 SCREEN CHARACTERISTICS

Explanations for the data appearing in the Dump Display appear below.

Rate - indicates either the Sample Rate, when the Internal Clock is being used, or External Clock, when an external source is being used as the sample clock. When Internal Clock is used, the Sample Rate is expressed in time units.

Delay - indicates the Delay (of Sample 0 compared to the Trigger Event), a data collection parameter specified on the Trigger Menu.

Window diagram - to the right of the Delay; shows where the samples displayed lie in the total 1000-sample trace memory.

SM or RM - to the right of window; indicate whether the data being displayed is in the Sample Memory or the Reference Memory. Selected via the Options Menu, O Command.

<G or G> - if shown, mean that there are glitches to the left or the right of the cursor. <G> indicates glitches to both the right and the left.

ref: - indicates the sample used as a reference point by the X Command, that is, the point from which an interval is measured. The X Command is a utility that calculates the interval, in number of samples and time, between two samples. See Section 16 for further information.

Enter: - shows the commands which may be entered next.

cur: - indicates the current cursor position in sample number or time units relative to the trigger event.

17.3 COMMAND FORMAT

The Dump Display is controlled by the D Command. Anytime the current display menu does not contain a D option, the data in trace memory may be displayed by using one of the following command formats:

Dx Display data in Dump format, starting from sample x.

D Display data in Dump format, centered on the current cursor position.

17.4 EXAMPLE

D16 Display data in Dump format, starting at sample 16.

17.5 DISPLAY CONTROL KEYS

The sample cursor is a highlighted "<" symbol. The sample marked by the cursor is also highlighted by intensified brightness. The cursor may be moved right, left, up, or down, or the entire display paged right or left, using these keys:

- < scroll the display horizontally one page to the left.
- > scroll the display horizontally one page to the right.
- <- move the cursor one column to the left.
- > move the cursor one column to the right.
- ↑ move the cursor up one sample.
- ↓ move the cursor down one sample.

17.6 HELP PAGE

To obtain the Help Page for the D Command, type "?D".

Rev. D

18. CORRELATION

18.1 INTRODUCTION

The Omni has a Sample Memory and a Reference Memory. The Reference Memory is normally used to hold data collected previously, for purposes of comparison with the data most recently collected.

The Correlation function makes the comparisons between data in the Sample and the Reference Memory. You can also use this function to define a scenario which data collection will be repeated until correlation with Reference Memory is attained; or until the sample data being collected fails to correlate with the reference data.

The Correlation function is controlled by the Correlation Menu, which appears in response to the C Command. Exhibit 18-1 shows an example of the Correlation Menu and of the resulting Correlation Display. Note that non-correlating samples are marked with a "<=>" symbol and highlighted.

This function is very effective for finding discrepancies between performance of a digital system under test (Sample) and a known good system (Reference).

In the simplest mode of operation, the <TAB> key (in conjunction with the Correlation Menu) causes correlation to be performed between the data in Sample and Reference Memories. It does not cause new data to be collected. Repeated use of the <TAB> key while viewing the Correlation Menu merely repeats the exercise of the correlation algorithm.

Correlation may be performed on the data in two disk files by following this procedure: first, call up the File Menu (F Command) and load one file into the Sample Memory using Item 4 or 5. Second, load the other file into Reference Memory using Item 3. Third, call up the Correlation Menu (C Command) and enter the desired correlation parameters on the menu. Next, press <TAB> to cause correlation to be performed. The result will be immediately displayed in a form similar to Exhibit 18-1(b).

18.2 CORRELATION MENU

Eight parameters are used to set the conditions for making correlations. The Correlation function has a number of modes that make it very flexible.

Item 1) File to correlate with:

The data in Reference Memory is loaded from a file on the disk. The file was created previously when data from a prior collection cycle was saved from the Sample Memory onto the disk, using the File Operations Menu.

```

1) File to correlate with: INTERNAL
                                F E D C B A 9 8 7 6 5 4 3 2 1 0
2) Channel mask:                1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
3) First sample included: 25
4) Number of samples: 400
5) Starting skew allowance: 25
6) Skew alignment samples: 1
7) Sampling tolerance: 5
8) Channel (bit) tolerance: 0
9) Repeat data collection until: A
   -> A) (not active)
       B) Samples correlate with reference
       C) Samples do not correlate with reference

```

Index 1-0, G to start, P, ?, or (space)

(a)

Ref #	Ref Data	Sam Data	Sam #
270	760F	760F	258
271	760F	<-> 761F	259
272	760F	760F	260
273	0038	0038	261
274	C239	C239	262
275	457A	457A	263
276	007B	007B	264
277	D105	D105	265
278	8F70	8F70	266
279	C071	C071	267
280	C806	C806	268
281	1807	1807	269
282	F848	F848	270
283	ED01	ED01	271
284	4F02	4F02	272
285	F803	F803	273
286	E904	E904	274
287	760E	760E	275
288	760F	760F	276
289	760F	760F	277
290	760F	760F	278
291	760F	760F	279

Correlation failed at sample: 271 -up, dn, (sp), P

(b)

Exhibit 18-1. Correlation Menu (a) and resulting display (b).

To retrieve the prior data from disk and load it into the Reference Memory, enter the filename in this item and press the return key. Alternatively, the file may be loaded to the Reference Memory using the File Menu (F Command). If the file is not on the disk, a disk I/O error message will appear. Recovery from the error is automatic; the input prompt will reappear at the lower left corner of the screen.

Item 2) Channel mask:

Channels which do not contain meaningful data and are to be ignored in the correlation can be "masked out" by entering a Channel Mask specification in Item 2. Enter a "1" to indicate channels to be included in the correlation. Enter an "X" to indicate channels to be excluded. If a "0" is entered, it will have the same effect as a "1". The cursor control keys -> and <- can be used to move the prompt-cursor without affecting a channel specification. Direct positioning of the prompt-cursor to Channels F through 2 can be accomplished by entering the channel number. Press <RETURN> or <SPACE> to leave this item.

Item 3) First sample included:

Item 3 allows you to specify the first sample at which the correlation process is to begin. Samples before the specified first sample are ignored by the correlation algorithm. The number entered here refers to the sample number in Reference Memory. The default entry for this item is Sample 0.

Item 4) Number of Samples:

This item is used in conjunction with Item 3 to limit the range of samples over which correlation is performed. The correlation algorithm will stop after processing the number of samples specified in this item.

Item 5) Starting point skew allowance:

Due to sampling differences, comparable patterns in the Sample and Reference Memory may not start at the same sample number. The difference is called "skew." The correlation algorithm allows for this skew. Item 5 may be used to specify the maximum allowable skew. For example, a value of 10 for the starting point and 4 for the skew would mean that starting point of the matching data in the Reference Memory could be anywhere from 6 to 14.

Item 6) Skew alignment samples:

The correlation skew algorithm begins comparing the data at a trial skew value, and if match is achieved over the number of samples specified in Item 6, it assumes that the trial skew value is correct. It then completes the comparison process and displays the result. If the correlation skew algorithm cannot locate a sequence of samples that match exactly for the specified skew alignment samples (and with a starting skew anywhere in the Item 5 skew allowance), then the correlation is aborted. If such is the case, an appropriate message is displayed.

For example, assume that 10 is entered in this item. Then when Sample and Reference Memory are compared using the trial skew value, if the first 10 samples compared match, the algorithm concludes that it has the correct skew value, completes the comparison, and displays the result.

If a match is not achieved over the first 10 samples, the algorithm tries another skew value. This process repeats until a skew value is found that gives a match over the first 10 samples, or all the skew values allowed by Item 5 have been tried.

The default value for this item is 1, which means that the algorithm tries different skew values until it finds one sample that matches, then it completes the correlation using that skew value.

Item 7) Sampling tolerance:

Sampling effects may cause some slight variation in the data collected, especially if you use Internal Clock, which is asynchronous with the system being measured. (Normally, External Clock is used.) Item 7 allows you to specify a Sampling Tolerance value; this is the number of nonmatching samples that will be allowed before correlation is considered to have failed.

When correlation fails, a message "Correlation failed at sample:" will appear at the bottom of the screen. If the Sampling Tolerance is 5, you will see 5 sample mismatches above the sample reported by the message as the one where correlation failed.

Item 8) Channel (bit) tolerance:

The channel (bit) error tolerance allows for the case where less than perfect correlation is desired. For example, correlating 14 channels out of 16 may be regarded as adequate. The number acceptable for a match, if different than the number of active channels as defined in the Channel Mask, may be specified in Item 8. Assuming that all 16 channels are active, then for this example it would be appropriate to enter 14 in Item 8.

Item 9) Repeat data collection until:

Selection A of this item is the default data collection mode. The Omni makes one data collection each time you issue the G Command or "=" Command.

When selection B is chosen, the Omni enters a mode in which it will collect data repeatedly. Then when you issue the G or "=" Command, the analyzer collects data to fill the Sample Memory, and then tests for correlation between the data just collected and the data in Reference Memory. If correlation is achieved, it stops and displays the result. If correlation is not achieved, it resumes data collection and then repeats the cycle. The process is repeated over and over until correlation is achieved.

Selection C also activates a repeat data collection mode. When you issue the G or "=" Command, the Omni likewise collects data to fill the Sample Memory, and then tests for correlation with the data in the Reference Memory. However, in this case, it continues to repeat the collect and correlate cycle so long as correlation is achieved; when correlation fails, it stops and displays the result.

Note that data is not being collected during the part of the cycle in which the Omni is testing for correlation in the data.

18.3 HELP PAGE

A Help Page for the Correlation Menu may be obtained by typing "?C". When viewing the menu, you can access Help Pages for Items 1, 2, etc., by typing "?1", "?2", etc. After seeing the help information, press <SPACE> to return to the Correlation Menu itself.

Rev. D

19. MATRIX DISPLAY

19.1 INTRODUCTION

This display, illustrated in Exhibit 19-1, is a table showing the number of times a specific bit pattern has occurred within a given range of samples. The maximum pattern length is eight bits. The display uses the lowest eight active channels according to the Trigger Menu, T Command.

Channels	7	6	5	4	3	2	1	0	Range	-500	to	499					
	0	1	2	3	4	5	6	7	8	9	A	B	C	D	E	F	
0	3	20	20	20	17	17	17							1	77	271	265
1	99														1	2	
2																	
3									21	20				3	3	3	3
4									17								
5																	
6																	
7	20	20												20	20		
8																	
9																	
A																	
B																	
C																	
D																	
E																	
F																	

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,sp

Exhibit 19-1. Matrix Display.

19.2 DISPLAY CHARACTERISTICS

There are 256 possible bytes, that is, 256 possible different combinations of 8 bits. The body of the table shows the number of times each of the 256 different combinations occurs in the specified range of samples.

A byte is represented in hexadecimal notation by two digits, e.g. "7B". The scale 0 - F on the left lists the first hex digit of the byte, and the scale across the top lists the second. Thus to find the number of occurrences of the byte "7B", find "7" on the left side scale, then read across to column "B". The example in Exhibit 19-1 shows that 7BH occurs 20 times.

The other features of the display are:

Channels - at the upper left; lists the eight (or less) channels that were surveyed in creating the display.

Range - at the upper right; gives the range of samples over which the count was made. In the example, the byte 7BH occurs 20 times between sample -500 and sample 499, inclusively. The range is specified in the parameters x and y used with the M Command.

Enter: - at the bottom; indicates the commands which are available now.

19.3 COMMAND FORMATS

The Matrix Diagram Display is controlled by the M Command by using one of the following command formats:

- M display matrix of data shown in previous display, starting from the same sample as the previous display. The number of samples shown will be the same as in the previous matrix.
- Mx display matrix of data for the same number of samples as the previous matrix, starting from sample x.
- Mx,y display matrix of data in Sample Memory from sample x to sample y, inclusively.
- MALL display matrix for entire Sample Memory.

The parameters x and y may be expressed as sample numbers. If Internal Clock is being used, they may be expressed either as sample numbers or as time units. When the Matrix Display is first used after turn-on, the default value for the number of samples over which the matrix is calculated is 80 samples; in other words, y is assumed equal to x+79 if it is not specified.

19.4 EXAMPLES

M16,64 display data between samples 16 and 64, inclusively.

M40ms display data starting at the sample 40 milliseconds after trigger, for the same number of samples as the previous display.

19.5 DISPLAY CONTROL KEYS

The "<" and ">" keys allow you to shift the range of samples over which the matrix is formed.

- < display matrix ranging over the same number of samples as the current matrix, but just before the current matrix.
- > display matrix ranging over the same number of samples as the current matrix, but just following the current matrix.

For example, assume that the current matrix is a summary over samples 40 through 79. Striking the "<" key causes a matrix for samples 0 through 39 to appear (after a short delay). The ">" key causes a matrix for samples 80 through 119 to appear.

19.6 HELP PAGE

To display the Help Page for the M Command, type "?M".

20. LOCATE

20.1 INTRODUCTION

Locate is a utility feature which finds a data pattern in the sampled data. It is used after data collection has occurred, and is independent of the Trigger Event and other trigger conditions used to specify the collection of data.

Exhibit 20-1 shows two examples of the Locate Menu, in which the search parameters are entered. Exhibit 20-2 shows the appearance of the Waveform Display after a desired sample pattern has been found and highlighted using the Locate function. Note that the cursor is on the sample containing "FC52", the first word of the Search Pattern specified in Exhibit 20-1(a).

20.2 LOCATE MENU

Enter "L" to bring up the Locate Menu. To change any aspect of the menu, enter the desired item number and change the parameter.

The first three items are used to set up conditions for the search. Item 1, Start Sample Number, indicates the sample number at which to begin the search. Item 2, Input Mode, specifies the number base for the subsequent items. Item 3, Global Channel Mask, is used to select the bits that will be used during the pattern search. Bits that are to be included in the search are indicated by a "1". Bits that are to be ignored are entered as a "0". The default conditions for these first three items are adequate for most searches.

The data pattern to be found is entered in Items 4 through 9, the Search Pattern. The pattern is a sequence of digital words which must be matched by a corresponding consecutive sequence of data samples in the Sample Memory. The search starts at the Start Sample Number and proceeds through the Sample Memory until the first complete match is found, or if there is no complete match, until it reaches the end of Sample Memory.

After entering the first word of the pattern in Item 4, press <RETURN> and the prompt-cursor will move to Item 5, ready to receive the second word. When you have entered as many words as your search pattern requires (often only one), press <SPACE> to leave the Search Pattern items.

20.3 MAKING THE SEARCH

When all changes to the menu have been entered, press the <TAB> key to initiate the pattern search. If the pattern is found, the Omni will return to a data display with the found pattern highlighted. If the pattern is not found, "Not Found" will appear in the upper right corner of the Locate Menu.

```

1) Start Sample Number -488
2) Input Mode          HEX

3) Global Channel Mask FFFF
4) Search Pattern      FC52
5)
6)
7)
8)
9)

```

Index 1-9, G to search, P, ?, or (space)

(a)

```

1) Start Sample Number -452
2) Input Mode          BINARY

                        F E D C B A 9 8 7 6 5 4 3 2 1 0
3) Global Channel Mask 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
4) Search Pattern      0 0 1 1 1 1 0 0 0 0 1 0 0 1 1 1
5)                    1 1 1 1 1 0 1 0 X X X X X X X X
6)                    X X X X X X X X X X X X X X X X
7)                    X X X X X X X X X X X X X X X X
8)                    0 0 0 0 1 0 0 0 X X X X X X X X
9)                    X X X X X X X X X X X X X X X X

```

Index 1-9, G to search, P, ?, or (space)

(b)

Exhibit 20-1. Locate Menu. (a) Example of entries in hexadecimal format. (b) Example of entries in binary format, which allows "don't care" ("X") specification of individual channels in the search pattern.

Item 1) Start Sample Number

A pattern search can begin at any sample within the 1000 sample trace. The sample can be specified either by a sample number, or if the Internal Clock is used, by a time value such as 50us or -1000ns. All sample number and time references are made with respect to the trigger event. Sample number 0 and time 0 normally correspond to the point at which the trigger event occurred. (If the Delay parameter, Item 8 on the Trigger Menu, is non-zero, then Sample 0 will be delayed relative to the trigger event by the Delay value chosen.)

When a starting sample number is selected, all samples before the starting sample are ignored when executing a pattern search.

Item 2) Input Mode

This item is used to select the most convenient number base for specifying the Channel Mask and Search Pattern. The default is hexadecimal. For binary, decimal, octal, or unsigned decimal, enter "B", "D", "O", or "U", respectively. "H" restores hexadecimal. When the Input Mode is changed, all lines following are automatically updated to reflect the new input number base.

Item 3) Global Channel Mask

Quite often a pattern search does not include all sixteen data channels. Through the use of the Global Pattern Mask, the unused channels can be ignored (made "don't care") during the search. A "1" indicates a channel that will be considered in the search. A "0" means "don't care", a channel that will be ignored in the search.

The Global Pattern Mask entry will usually be in a number base other than binary, such as hexadecimal. In that case, the pattern of "1"'s and "0"'s just mentioned refers to the binary form of the number (as is always the case when a number is used to describe digital signals).

When the Search Pattern is specified in a number base other than binary, the Global Pattern Mask is the only way to indicate specific "don't care" channels. When the Input Mode is binary, as an alternative each "don't care" channel can be indicated with an "X" in the Search Pattern.

Items 4) thru 9) Search Pattern

The Search Pattern can consist of one to six consecutive sixteen bit words. The search is considered successful only if a consecutive sequence of samples is found in the Sample Memory that matches the pattern word for word. "Don't care" patterns are indicated by a blank line, and are entered by pressing <RETURN> to skip over the line. When in binary mode, a "don't care" pattern can be entered with an "X" on every channel. Upon completion of the pattern entry, press <SPACE> to exit this item.

20.5 EXAMPLES

The first example involves monitoring the instruction sequence on a microprocessor's eight-bit data bus. Consider the menu entries:

- 1) Start Sample Number 50
- 2) Input Mode HEX
- 3) Global Channel Mask FF00
- 4) Pattern C300
- 5) 5500
- 6) 2300
- 7)
- 8)
- 9)

Here the channels of interest are the upper 8 (i.e., Channels F through 8). This is indicated by eight high level bits ("FF") in the top (leftmost) position of the Global Channel Mask. The lower eight bits of the Global Channel Mask are set to "0" to establish a "don't care" condition on the low channels.

The pattern is the sequence "C3", "55", and "23". (I.e., a jump to location 2355 on a Z80 microprocessor. The "55" comes before the "23" because the Z80 fetches the low byte first.) To maintain positional integrity, each of these three entries was filled to the right with "00". (Any eight-bit fill would provide the same result because the Channel Mask forces these bits to be "don't cares" during the search.) Because the start sample number is 50, any occurrences of the three sample sequence before sample number 50 are ignored.

The second example illustrates the same application scenario, however the search is generalized to require a match on any jump to a 23XX address. The menu entries for this case are:

- 1) Start Sample Number 50
- 2) Input Mode BINARY
- 3) Global Channel Mask 1 1 1 1 1 1 1 1 X X X X X X X X
- 4) Pattern 1 1 0 0 0 0 1 1 X X X X X X X X
- 5) X X X X X X X X X X X X X X X X
- 6) 0 0 1 0 0 0 1 1 X X X X X X X X
- 7)
- 8)
- 9)

Since the input mode is binary, additional qualification of the pattern is possible. The Global Channel Mask specification forces the use of only the high eight bits in the search. The second sample in the pattern is specified as a "don't care", and hence will always match the data collected following the "C3". The search will be successful on any

three sample sequence where the first sample is "C3", the third is "23" and the second can be any pattern.

20.6 HELP PAGE

A Help Page for the Locate Menu may be accessed with "?L". When viewing the menu itself, you can access Help Pages for the individual Items 1, 2, etc., by typing "?1", "?2", etc. Press <SPACE> to return to the Locate Menu from the Help Pages.

Kaypro Journal

Rev. D

21. FILE OPERATIONS

21.1 INTRODUCTION

File operations allow you to:

- o store and retrieve sample data and test parameters to and from disk files.
- o display a directory of the files stored on disk.
- o delete data files.
- o move data from Sample Memory to Reference Memory.
- o retrieve tables of instruction mnemonics for different microprocessors for the Instruction Disassembly function.
- o record keystrokes in a log file, and later re-execute them automatically.

These functions are controlled by the File Menu, which appears in response to the F Command. Exhibit 21-1 shows the File Menu as it appears when first called up.

21.2 MENU ITEMS

Explanations of the individual menu items follow.

Item 1) Title:

The title is an optional input of up to 40 characters which will label any individual data or setup parameter file saved on disk. When this stored data is retrieved, the title is also displayed. The use of a title is a convenient way to describe the characteristics of the recorded data file for positive identification at a later time.

NOTE: Spaces are not allowed in the title. Use the underscore character or hyphen instead.

Item 2) READ instruction MNEMONICS from file:

Instruction disassembly is performed by matching collected data with a predefined file of instruction mnemonics. Some mnemonics have already been defined and recorded on disk under files bearing the name of the processor and the file extension ".LAM". When specifying the filename in Item 2, enter only the name of the file; the extension is appended automatically.

```

1) Title:

2) READ instruction MNEMONICS from file: Z80      LAM
3) READ into REFERENCE memory from file:
4) READ into SAMPLE memory from file:
5) READ ALL data & parameters from file:

6) WRITE SAMPLE memory onto file:
7) WRITE ALL data & parameters onto file:

8) Display DIRECTORY of saved files on drive: A
9) DELETE data file:
A) COPY from SAMPLE into REFERENCE memory
B) Log file status:      TEST87 LAL
Collection dates:      Sample      Reference
                       08/07/84 16:42:15  08/07/84 16:39:18

```

Enter 1 - B, ? for help, or SPACE to exit

Exhibit 21-1. File Menu. The Z80 mnemonics file, which is used for Instruction Disassembly, appears by default in Item 2.

Item 3) READ into REFERENCE memory from file:

After sample data has been collected and saved on disk, it can be returned to either Sample or Reference Memory. Moving stored data into Reference Memory allows it to be displayed just like data in Sample Memory, or it can be used for Correlation operations. Data is read from disk into Reference Memory when the filename is entered in this item and the <RETURN> key pressed. Do not enter an extension; the extension ".LAD" is appended automatically.

NOTE: The preceding function will not provide Reference Signatures for signature analysis. They must be read in using Item 7 on the Signature Menu. See Section 24, Signature Analysis.

Item 4) READ into SAMPLE memory from file:

To transfer data from a disk file to the Sample Memory, enter the filename (without the extension) in this item. The data will be restored in its raw format and will not contain any characteristics such as channel labels, Sample Rates, or trigger conditions. When the retrieved data is displayed, the time scale and other collection

parameters on the screen may not correspond to the data, and a warning message to that effect will be displayed.

The Omni records date and time when sample data is collected. This time record is saved with a stored file, and returned when the file is returned.

Item 5) READ all data & parameters from file:

This item retrieves data and parameters that were saved using Item 7. Upon retrieval of the data and parameters, the analyzer setup conditions (trigger word, display number base, etc.) are totally reconfigured from their current state to the setup conditions that were saved on disk. Use of this option is a convenient way to restore a given setup state from a power-up condition.

NOTE: All the parameter settings currently in effect will be lost when this function is used, since it replaces them with the parameters stored on disk. This includes changing the data in Reference Memory, if File Menu Item 3 had a filename in it when the analyzer state was originally stored via Item 7.

CAUTION: Data files saved using earlier versions of the Logic Analyzer Program should not be recalled using this item. In order to expand capabilities, it was necessary to modify the parameter storage formats. As a result, attempting to recall data that was saved using an early program version (prior to 4-1-84) may cause problems.

Item 6) WRITE SAMPLE memory onto file:

After data collection has been made, the data can be saved to a disk file by entering the filename in this item. Filenames can contain up to eight alphanumeric characters and an optional disk drive specifier in the standard format:

d:ffffff

where d is the drive specifier ("A" or "B") and fffffff is the filename. Do not enter an extension; all files saved will be automatically assigned the extension ".LAD".

If the disk drive specifier is omitted, the specifier for the default drive (often called the logged in drive) will be supplied automatically. If a drive other than the current default drive is specified, then the specified drive will become the new default drive. The default drive is displayed on the File Menu in Item 8.

Item 7) WRITE ALL data & parameters onto file:

Item 7 allows you to save not only the data, but also the setup conditions of the analyzer. Channel labels, trigger conditions, Sample Rates, and display parameters (the total state of the machine) are all saved to disk. The former setup conditions (the entire state) are restored through the use of Item 5. Enter the filename as in Item 6.

Item 8) Display DIRECTORY of save files on drive: A

It is difficult to remember all the file names that have been saved on a particular disk. To display a list of the logic analyzer files resident on a given disk, select this item and enter the drive letter ("A" or "B") of the desired drive.

Press any key other than <SPACE> to see a display of all the files on the disk. After viewing the directory, press <SPACE> to return to the File Menu.

Item 9) DELETE data file:

Enter the name of a file (less the extension) in this item to delete it from the disk.

Item A) COPY from SAMPLE into REFERENCE memory:

Accessing this item causes data to be copied from the Sample Memory to the Reference Memory. Typically, a new sample collection will then be made for comparison to the previous data. The Correlation function, for example, correlates data in Sample Memory against data in Reference Memory.

Item B) Log file status:

This item is used to make a log of your keystrokes which is saved in a disk file. The keystroke sequence may be recalled and automatically re-executed at a later time.

To create a log file, type "B" to access this item. Then enter "W" for "write to log file." Enter the filename (less the extension) when prompted for it. After the filename is entered, all keystrokes will be recorded automatically.

To end the logging of keystrokes, type "B" to access this item again. The Log file status will be immediately changed back to Inactive.

To re-execute the recorded keystrokes, access this item and type "R", for "read from log file", when prompted. Then enter the filename of the desired log file. After you have entered the filename, the Omni will fetch the file and re-execute the keystroke sequence it contains as you watch. When it reaches the end of the file, the Log file status will be reset to Inactive.

21.3 HELP PAGE

A Help Page for the File Menu may be accessed by typing "?F". When viewing the Menu, you can obtain Help Pages for the individual Items 1, 2, etc., by typing "?1", "?2", and so on. After viewing a Help Page, press <SPACE> to return to the File Menu itself.

Rev. D

22. INSTRUCTION DISASSEMBLY

22.1 INTRODUCTION

A microprocessor executes its program by fetching instructions and data from memory. The instructions are made up of two parts, opcodes and operands. They appear as bit patterns on the data bus when the microprocessor reads them from memory.

The Instruction Disassembly function allows you to trace program flow by collecting this data bus activity and translating the bit patterns back into instruction mnemonics.

To effectively utilize this mode of display, a very controlled data collection procedure must be observed. This requires coordination between the selection of channels, mnemonic definitions in a disk file, and selection of an appropriate External Clock source.

The disassembler operates on the data in eight channels, corresponding to the data bus of eight-bit microprocessors. The optional 32 Channel Adapter, which extends the Omni's data collection capability to 32 channels total, makes possible collection of complete data and address activity.

Use of the Omni's internal clock is not appropriate for instruction disassembly, since it is not synchronized with the data on the microprocessor's data bus. The data bus is time shared, and valid data is present only while certain control lines are valid. Use one of these control lines as the External Clock signal to record data into the logic analyzer's memory, for example the "MEMORY READ" control line. Be aware of the polarity of the control signal selected for use as the External Clock. The Omni collects data on the edge of the External Clock signal.

Once the setup requirements and precautions have been observed, and valid data collected, displaying the information in instruction format is easy. The I Command initiates instruction disassembly.

NOTE: The I Command does not cause a new sample to be collected; it merely translates the data already in Sample Memory into mnemonics.

22.2 DISPLAY FORMAT

After disassembly, the data is displayed as both bit patterns and mnemonics in a format similar to that obtained from an assembler listing. Exhibit 22-1 shows an example of the Instruction Disassembly display.


The display is made up of several columns of data. The left column is the sample number ("-465" in the first line in Exhibit 22-1). The middle columns are the collected data ("00001111-CB" in the exhibit). The right column shows the collected data translated into mnemonics ("BIT 0,(HL)").

Sample	D0-D7 Ctrl Bits, D8-DF Bytes	Mnemonic	D0-DF Bytes
-465	00001111-CB	00010000-46	BIT 0, (HL) C0
-462	00010001-28	01010010-FC	JR Z, FC
-460	00001111-CB	00010000-46	BIT 0, (HL) C0
-457	00010001-28	01010010-FC	JR Z, FC
-455	00001111-CB	00100110-08	RRC B
-> -453	00100111-3C		INC A
-452	00101000-FA	00000000-6D	JP M, 006D
-449	00101101-08		EX AF, AF*
-448	00101110-C3		RET CF 04
-445	00001111-CB	00010000-46	BIT 0, (HL) C0
-442	00010001-28	01010010-FC	JR Z, FC
-440	00011111-CB	00010000-46	BIT 0, (HL) C0
-437	00010001-28	01010010-FC	JR Z, FC
-435	00001111-CB	00010000-46	BIT 0, (HL) C0
-432	00010001-28	01010010-FC	JR Z, FC
-430	00001111-CB	00010000-46	BIT 0, (HL) C0
-427	00010001-28	01010010-FC	JR Z, FC
-425	00001111-CB	00010000-46	BIT 0, (HL) C0
-422	00010001-28	01010010-FC	JR Z, FC
-420	00001111-CB	00010000-46	BIT 0, (HL) C0
-417	00010001-28	01010010-FC	JR Z, FC
-415	00001111-CB	00010000-46	BIT 0, (HL) C0

Enter: C, D, E, F, G, H, I, L, M, N, O, P, S, T, W, X, Z, =, ?, sp

Exhibit 22-1. Instruction Disassembly Display. The I Command causes data in the Sample Memory to be displayed as instruction mnemonics.

The collected data "00001111-CB" is displayed in this format:

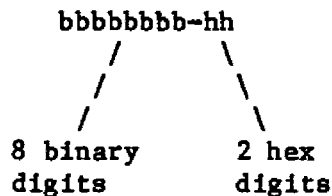

The 8 bits bbbbbb represent the signals on Omni Channels 7-0, some of which are connected to the microprocessor control lines. The two hex digits represent the data collected on Omni Channels F-8, which are connected to the microprocessor data bus.

Each line of the display corresponds to one instruction of disassembled code. Each line will have either one or two of the bbbbbbb-hh patterns, depending on whether the instruction is a one-byte or multibyte instruction. For instructions longer than two bytes, the bbbbbbb-hh patterns show only the first two bytes.

The representation of the Channel 7-0 control bits (bbbbbbb) is always in binary. The number base for the Channel F-8 data bytes (hh) is dictated by the Options Menu, reached by the O Command. The default output base is hexadecimal. Refer to the Options Menu section for the procedure to change the output base.

As well as mnemonics, the last column also shows any bytes which are read by the microprocessor when it executes the instruction. For example, look at the instruction starting at Sample -448. The instruction "RET" is a single-byte instruction; "C9" is the opcode. To execute the instruction, the microprocessor read bytes "CF" and "04" from memory.

Thus the last column shows all data bus activity - both the reading of the instruction and its execution.

As with the other display formats, the cursor keys can be used to move the highlighted cursor up or down, or scroll the entire display.

22.3 HOW IT WORKS

During program execution, not only instructions appear on the data bus; data read from memory and (in the case of processors using memory-mapped I/O) input data appear as well. The disassembler must be able to distinguish the opcode bytes from all the others in order to disassemble the code correctly. There are three ways to do this:

Use the status lines - some processors provide status signals that identify the opcode fetches. The Z80's /MREQ and /M1 signals do this, and the Omni's built-in Z80 disassembler uses them. The 8085 and 8080 provide status signals /IOM, S0, and S1, which the Omni uses.

Start from a known opcode - if status signals are not available, a non-status disassembler will work properly if it is started on an opcode. The Omni's other disassemblers work this way. You should start disassembly from an opcode byte with the command "I n", where sample n contains an opcode.

Start anywhere - if a disassembler of the second type is started on a byte which is not an opcode, the disassembler will erroneously interpret it as an opcode and display incorrect instructions. However, after a few lines of disassembly, it will strike an opcode, get "in sync", and disassemble correctly from there on.

The Omni actually contains two disassemblers: a status signal type disassembler with built-in mnemonics for the Z80 and 8085, and a table driven disassembler that reads in the mnemonics from a file and can be

used with any processor. The two disassemblers work somewhat differently, so they will be described separately.

22.4 Z80 INSTRUCTION DISASSEMBLY

The Z80 Disassembly is the default choice - it is activated when you first use the I Command. Reading a mnemonic file via the File Menu is not required.

To perform disassembly for a Z80 microprocessor, first connect Channels F-8 of the Omni to the Z80 data lines D7-D0 respectively.

Note: The symbols "D7", "D6", and so on are used for two different applications - Omni probe lines and microprocessor data bus signals. To avoid confusion here, we will refer to the Omni input lines as "Channel F", "Channel 7", and so on. In this section of the manual, "D7", "D6", etc. are used only to refer to the microprocessor data bus.

Connect /MREQ and /M1 to Omni Channels 6 and 7, respectively. These are the two lines that are recorded to distinguish opcode fetches from other bus activity. Attach the Clock probe lead to the microprocessor system /RD line.

Set up the desired data collection parameters on the Trigger Menu. Use the External Clock option and clock on the positive edge. Use the Latched Mode.

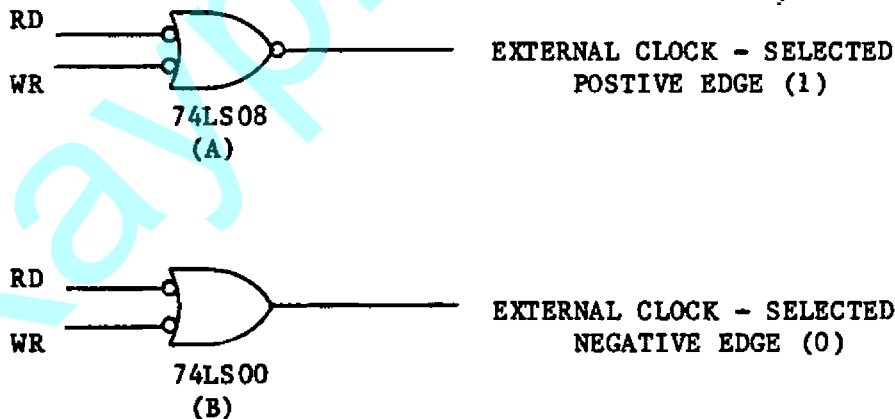


Exhibit 22-2. Circuits to combine /RD and /WR microprocessor strobe signals into a single External Clock pulse. This allows both read and write bus cycles to be recorded, and thus appear in the Instruction

After all desired trigger parameters are set up and data has been collected, enter the command "I<RETURN>" to perform instruction disassembly. A display similar to Exhibit 22-1 will appear. Move the cursor by using the up and down arrow keys, and step pages by using the "<" and ">" keys.

The six channels not connected yet, Channels 5 through 0, will also be displayed in binary form in the second column, along with Channels 7 and 6. They may be used to monitor any other signals you wish, such as address lines or bits of I/O ports. Remember, a maximum of two bus cycles per opcode fetch will be displayed for these lines. The Dump display may be used to observe any bus cycles for Channels 7-0 not shown by the Instruction Disassembly display, although this is rarely required.

If it is required that data from write and output cycles be recorded in disassembly, then an external gate will be required to logically-OR the /RD and /WR lines to the External Clock input. Exhibit 22-2 on the previous page shows two possible circuits to accomplish this.

22.5 8085/8080 DISASSEMBLY

Mnemonics for the 8085/8080 family microprocessors are also available. The 8085 is a single-chip improved version of the 8080. It runs the same software, except that it has two added instructions the 8080 does not have. The status signals are the same, /IOM, S0, and S1.

To activate the 8085/8080 mnemonics, enter 8085 in Item 2 on the File Menu. Note that no mnemonics files for these processors will appear in the disk directory - like the Z80 mnemonics, they are built into the disassembler.

Connect Channels F-8 of the Omni to the microprocessor's data lines 7 through 0, respectively. The latter are labeled AD7-AD0 on 8085 and 8080 chip set diagrams. Connect Channel 7 to microprocessor status line /IOM, Channel 6 to status line S0, and Channel 5 to status line S1.

From this point, proceed as recommended above for the Z80.

22.6 FILE DRIVEN DISASSEMBLER

The file-driven disassembler does not require status signals from the microprocessor. It finds opcodes by the "start from a known opcode" or "start anywhere" methods.

To load the mnemonics for a given microprocessor, first call up the File Menu with the F Command. Enter the name of the file containing the mnemonics for the processor you wish to use in Item 2, Read Instruction Mnemonics From File. Mnemonic files are stored on disk with the file extension ".LAM". (Do not type the extension; ".LAM" will be appended to the file name automatically.)

After the data has been collected, use the I Command to initiate disassembly. If you know that sample n contains an opcode, you can type "In<RETURN>" and disassembly will be correct starting from sample n. Often, however, you will not initially know which samples contain opcodes. In that case, the first few lines of disassembled code will be incorrect.

22.7 8048 SERIES FILE DRIVEN DISASSEMBLY

The following briefly explains how to perform instruction disassembly for the 8048 Series microcomputers (8048, 8748, 8039, 8035, 80C48, etc.). A general knowledge of this family of microcomputers is assumed. The file-driven disassembler is used with this series.

A special requirement of 8048 Series disassembly is that the microcomputer be executing its program from external ROM, since this is the only time opcodes are present on the data bus and can be captured. PSEN (pin 9) will be used to strobe the data in, so connect this line to the Omni's External Clock (positive edge). Connect the 8 data lines from the microcomputer chip (pins 12-19) to Channels F-8 on the Omni.

Set up the trigger conditions as needed. The mnemonics file for the 8048 series is stored on the Logic Analyzer disk under the name 8048FAM.LAM. Load it using Item 2 on the File Menu. At this point data can be collected and the I Command can be used to disassemble the code.

The lower 8 channels (Channels 7-0) are not required for disassembly and may all be used for other functions, such as monitoring addresses or bits from I/O ports. These channels are displayed in binary form.

As was noted above, this approach is based on a method of collecting data only when PSEN is active. The mnemonics table in the file 8048.FAM is constructed for this method, and if you wish to use a different approach, you will need to change the table.

22.8 CREATING MNEMONICS FILES FOR OTHER PROCESSORS

You can disassemble code for any processor or state sequencer by putting a table of the corresponding mnemonics in a file on disk. Exhibit 22-3 specifies the construction of the table. This makes it possible to add instruction disassembly capability for new processors - it is only necessary to construct a new table.

The first two bytes in the file represent the size of the table (including the first two bytes). Next follow 256 packets, one for each of the 256 possible one-byte opcodes. Unused opcodes must also be represented in the file, with the mnemonic "??" (two question marks) assigned to them.

The lead byte in the first packet (labeled "byte 2" in Exhibit 22-3) is a binary number that equals the number of bytes in the packet (including the first byte). The next byte ("byte 3") is a binary number representing the number of bytes in the instruction fetch for the instruction; this is normally one. The next byte ("byte 4") is the

number of bytes of operand fetch and additional bus cycles that the processor executes for the instruction. The next byte ("byte 5") is the opcode, that is, the machine code binary number. The remaining bytes in the packet ("bytes 6, 7, ... n") are the ASCII codes for the instruction mnemonic.

Subsequent packets are constructed the same way. Note that the packets are of varying length, depending on the number of bytes (characters) in the mnemonic. The next packet follows immediately after the end of the prior packet; there is no delimiter between packets. The disassembler subroutine uses the first byte of each packet to tell where the next packet starts.

DESCRIPTION OF MNEMONICS TABLE

byte 0,1 = size of table (unused by online disassembly)

PACKET DESCRIPTION

byte 2 = number of bytes in packet
byte 3 = number of bytes of instruction fetch
byte 4 = number of bytes of operands fetch and additional bus cycles
byte 5 = opcode
byte 6,7,...,m = ASCII for instruction mnemonic

NEXT PACKET DESCRIPTION

byte m+1 = number of bytes to describe 2nd packet etc.
:
:
:

TERMINATOR BYTE DESCRIPTION

byte n = 0 to signal end of table

DESCRIPTION OF PACKET FOR UNDEFINED OPCODES

byte j+1 = 6
byte j+2 = 1
byte j+3 = 0 (zero)
byte j+4 = opcode
byte j+5, j+6 = 63, 63 = ASCII for "??" (two question marks)

Exhibit 22-3. Instruction Disassembly Mnemonic Table Specification. This describes the structure of the mnemonics table used in disassembly. You must have a table like this for every processor for which disassembly is to be performed. (Except the Z80 and 8085, for which the disassembler has mnemonics built in.) The maximum size allowed for this table is 3K bytes.

After the 256 packets for the possible opcodes, a terminator byte marks the end of the table. It is simply one byte containing a binary zero (0). Note that the maximum size allowed for the table is 3K bytes.

Since the file is a binary file, you need to use an assembler or some other program that will produce binary output to create it. We suggest that you use an editor to make an .ASM file, then use ASM and LOAD to make hex and binary versions. Rename the binary version of the file to change its extension from ".COM" to ".LAM".

Exhibit 22-4 at the end of this section shows the mnemonics table (in the form of an .ASM file) for the 8048 microprocessor.

22.9 COMMAND FORMAT

Anytime the prompt line

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,(sp),^P

appears, the data in trace memory may be displayed in Instruction Disassembly mode using a command in the following format:

- I Display data in Disassembled Instruction format, centered on the sample marked with the cursor in the previous display.
- Ix Display data in Disassembled Instruction format starting from sample number x.

22.10 COMMAND EXAMPLE

I56 Display data as disassembled instructions starting at sample number 56.

22.11 HELP PAGE

To obtain the Help Page for this function, type "?I".

DISASSEMBLY SOURCE

```

DW      TBLEND          ;END OF TABLE

DB      007H,01,00,00,'NOP'
DB      006H,01,00,01,'???'
DB      00EH,01,00,02,'OUTL BUS,A'
DB      00BH,01,01,03,'ADD A,#'
DB      010H,01,01,04,'JMP PAGE 0,#'
DB      007H,01,00,05,'ENI'
DB      006H,01,00,06,'???'
DB      009H,01,00,07,'DEC A'
DB      00EH,01,00,08,'INS A, BUS'
DB      00BH,01,00,09,'IN A,F1'
DB      00EH,01,00,0AH,'IN A,F2'
DB      006H,01,00,0BH,'???'
DB      00DH,01,00,0CH,'MOVD A,F4'
DB      00DH,01,00,0DH,'MOVD A,F5'
DB      00DH,01,00,0EH,'MOVD A,F6'
DB      00DH,01,00,0FH,'MOVD A,F7'
DB      00BH,01,00,10H,'INC @R0'
DB      00BH,01,00,11H,'INC @R1'
DB      007H,01,01,12H,'JRO'
DB      00CH,01,01,13H,'ADDC A,#'
DB      011H,01,01,14H,'CALL PAGE 0,#'
DB      009H,01,00,15H,'DIS I'
DB      007H,01,01,16H,'JTF'
DB      009H,01,00,17H,'INC A'
DB      00AH,01,00,18H,'INC R0'
DB      00AH,01,00,19H,'INC R1'
DB      00AH,01,00,1AH,'INC R2'
DB      00AH,01,00,1BH,'INC R3'
DB      00AH,01,00,1CH,'INC R4'
DB      00AH,01,00,1DH,'INC R5'
DB      00AH,01,00,1EH,'INC R6'
DB      00AH,01,00,1FH,'INC R7'
DB      00DH,01,00,20H,'XCH A,@R0'
DB      00DH,01,00,21H,'XCH A,@R1'
DB      006H,01,00,22H,'???'
DB      00BH,01,01,23H,'MOV A,#'
DB      010H,01,01,24H,'JMP PAGE 1,#'
DB      00CH,01,00,25H,'EN TCNT1'
DB      00BH,01,01,26H,'JNTO'
DB      009H,01,00,27H,'CLR A'
DB      00CH,01,00,28H,'XCH A,R0'
DB      00CH,01,00,29H,'XCH A,R1'
DB      00CH,01,00,2AH,'XCH A,R2'
DB      00CH,01,00,2BH,'XCH A,R3'
DB      00CH,01,00,2CH,'XCH A,R4'
DB      00CH,01,00,2DH,'XCH A,R5'
DB      00CH,01,00,2EH,'XCH A,R6'
DB      00CH,01,00,2FH,'XCH A,R7'
DB      00EH,01,00,30H,'XCHD A,@R0'
DB      00EH,01,00,31H,'XCHD A,@R1'
DB      007H,01,01,32H,'JBI'
DB      006H,01,00,33H,'???'
DB      010H,01,01,34H,'CALL PAGE 1#'
DB      00DH,01,00,35H,'DIS TCNT1'
DB      007H,01,01,36H,'JTO'
DB      009H,01,00,37H,'CPL A'
DB      006H,01,00,38H,'???'
DB      00DH,01,00,39H,'OUTL P1,A'
DB      00DH,01,00,3AH,'OUTL P2,A'
DB      006H,01,00,3BH,'???'

DB      00DH,01,00,3CH,'MOVD F4,A'
DB      00DH,01,00,3DH,'MOVD F5,A'
DB      00DH,01,00,3EH,'MOVD F6,A'
DB      00DH,01,00,3FH,'MOVD F7,A'
DB      00DH,01,00,40H,'ORL A,@R0'
DB      00DH,01,00,41H,'ORL A,@R1'
DB      00BH,01,00,42H,'MOV A,T'
DB      00BH,01,01,43H,'ORL A,#'
DB      010H,01,01,44H,'JMP PAGE 2,#'
DB      00CH,01,00,45H,'STRT CNT'
DB      00BH,01,01,46H,'JNT1'
DB      00AH,01,00,47H,'SWAP A'
DB      00CH,01,00,48H,'ORL A,R0'
DB      00CH,01,00,49H,'ORL A,R1'
DB      00CH,01,00,4AH,'ORL A,R2'
DB      00CH,01,00,4BH,'ORL A,R3'
DB      00CH,01,00,4CH,'ORL A,R4'
DB      00CH,01,00,4DH,'ORL A,R5'
DB      00CH,01,00,4EH,'ORL A,R6'
DB      00CH,01,00,4FH,'ORL A,R7'
DB      00DH,01,00,50H,'ANL A,@R0'
DB      00DH,01,00,51H,'ANL A,@R1'
DB      007H,01,01,52H,'JB2'
DB      00BH,01,01,53H,'ANL A,#'
DB      011H,01,01,54H,'CALL PAGE 2,#'
DB      00AH,01,00,55H,'STRT T'
DB      007H,01,01,56H,'JTI'
DB      00BH,01,00,57H,'DA A'
DB      00CH,01,00,58H,'ANL A,R0'
DB      00CH,01,00,59H,'ANL A,R1'
DB      00CH,01,00,5AH,'ANL A,R2'
DB      00CH,01,00,5BH,'ANL A,R3'
DB      00CH,01,00,5CH,'ANL A,R4'
DB      00CH,01,00,5DH,'ANL A,R5'
DB      00CH,01,00,5EH,'ANL A,R6'
DB      00CH,01,00,5FH,'ANL A,R7'
DB      00CH,01,00,60H,'ADDA,@R0'
DB      00CH,01,00,61H,'ADDA,@R1'
DB      00BH,01,00,62H,'MOV T,A'
DB      006H,01,00,63H,'???'
DB      010H,01,01,64H,'JMP PAGE 3,#'
DB      00DH,01,00,65H,'STOP TCNT'
DB      006H,01,00,66H,'???'
DB      009H,01,00,67H,'RRR A'
DB      00CH,01,00,68H,'ADD A,R0'
DB      00CH,01,00,69H,'ADD A,R1'
DB      00CH,01,00,6AH,'ADD A,R2'
DB      00CH,01,00,6BH,'ADD A,R3'
DB      00CH,01,00,6CH,'ADD A,R4'
DB      00CH,01,00,6DH,'ADD A,R5'
DB      00CH,01,00,6EH,'ADD A,R6'
DB      00CH,01,00,6FH,'ADD A,R7'
DB      00EH,01,00,70H,'ADDC A,@R0'
DB      00EH,01,00,71H,'ADDC A,@R1'
DB      007H,01,01,72H,'JB3'
DB      006H,01,00,73H,'???'
DB      011H,01,01,74H,'CALL PAGE 3,#'
DB      00CH,01,00,75H,'ENTO CLK'
DB      007H,01,01,76H,'JF1'
DB      00BH,01,00,77H,'RR A'
DB      00DH,01,00,78H,'ADDC A,R0'
DB      00DH,01,00,79H,'ADDC A,R1'
DB      00DH,01,00,7AH,'ADDC A,R2'
DB      00DH,01,00,7BH,'ADDC A,R3'
DB      00DH,01,00,7CH,'ADDC A,R4'
DB      00DH,01,00,7DH,'ADDC A,R5'

```

Exhibit 22-4. Mnemonics table for the 8048 microprocessor. This is an assembly language source file, designed to be assembled using ASM, the Digital Research assembler supplied with CP/M. This listing is provided here as an example; the compiled file is included on the Logic Analyzer Disk as 8048FAM.LAM.

```

DB 00DH,01,00,7EH,'ADDC A,R6'
DB 00DH,01,00,7FH,'ADDC A,R7'
DB 00EH,01,01,80H,'MOVX A,@R0'
DB 00EH,01,01,81H,'MOVX A,@R1'
DB 006H,01,00,82H,'???'
DB 007H,01,00,83H,'RET'
DB 010H,01,01,84H,'JMP PAGE 4, #'
DB 00AH,01,00,85H,'CLR F0'
DB 007H,01,01,86H,'JNZ'
DB 006H,01,00,87H,'???'
DB 00DH,01,01,88H,'DRL BUS, #'
DB 00CH,01,01,89H,'DRL F0, #'
DB 00CH,01,01,8AH,'DRL F1, #'
DB 006H,01,00,8BH,'???'
DB 00DH,01,00,8CH,'DRLD F4, A'
DB 00DH,01,00,8DH,'DRLD F5, A'
DB 00DH,01,00,8EH,'DRLD F6, A'
DB 00DH,01,00,8FH,'DRLD F7, A'
DB 00EH,01,01,90H,'MOVX @R0, A'
DB 00EH,01,01,91H,'MOVX @R1, A'
DB 007H,01,01,92H,'JB4'
DB 008H,01,00,93H,'RETF'
DB 011H,01,01,94H,'CALL PAGE 4, #'
DB 00AH,01,00,95H,'CPL F0'
DB 007H,01,01,96H,'JNZ'
DB 009H,01,00,97H,'CLR C'
DB 00DH,01,01,98H,'ANL BUS, #'
DB 00CH,01,01,99H,'ANL F1, #'
DB 00CH,01,01,9AH,'ANL F2, #'
DB 006H,01,00,9BH,'???'
DB 00DH,01,00,9CH,'ANLD F4, A'
DB 00DH,01,00,9DH,'ANLD F5, A'
DB 00DH,01,00,9EH,'ANLD F6, A'
DB 00DH,01,00,9FH,'ANLD F7, A'
DB 00DH,01,00,0A0H,'MOV @R0, A'
DB 00DH,01,00,0A1H,'MOV @R1, A'
DB 006H,01,00,0A2H,'???'
DB 00DH,01,00,0A3H,'MOV @R0, A'
DB 010H,01,01,0A4H,'JMP PAGE 5, #'
DB 00AH,01,00,0A5H,'CLR F1'
DB 006H,01,00,0A6H,'???'
DB 009H,01,00,0A7H,'CPL C'
DB 00CH,01,00,0A8H,'MOV R0, A'
DB 00CH,01,00,0A9H,'MOV R1, A'
DB 00CH,01,00,0AAH,'MOV R2, A'
DB 00CH,01,00,0ABH,'MOV R3, A'
DB 00CH,01,00,0ACH,'MOV R4, A'
DB 00CH,01,00,0ADH,'MOV R5, A'
DB 00CH,01,00,0AEH,'MOV R6, A'
DB 00CH,01,00,0AFH,'MOV R7, A'
DB 00DH,01,01,0B0H,'MOV @R0, #'
DB 00DH,01,01,0B1H,'MOV @R1, #'
DB 007H,01,01,0B2H,'JB5'
DB 008H,01,00,0B3H,'JMPP @A'
DB 011H,01,01,0B4H,'CALL PAGE 5, #'
DB 00AH,01,00,0B5H,'CPL F1'
DB 007H,01,01,0B6H,'JF0'
DB 006H,01,00,0B7H,'???'
DB 00CH,01,01,0B8H,'MOV R0, #'
DB 00CH,01,01,0B9H,'MOV R1, #'
DB 00CH,01,01,0BAH,'MOV R2, #'
DB 00CH,01,01,0BBH,'MOV R3, #'
DB 00CH,01,01,0BCH,'MOV R4, #'
DB 00CH,01,01,0BDH,'MOV R5, #'
DB 00CH,01,01,0BEH,'MOV R6, #'
DB 00CH,01,01,0BFH,'MOV R7, #'

```

TABLEND:

```

DB 006H,01,00,0C0H,'???'
DB 006H,01,00,0C1H,'???'
DB 006H,01,00,0C2H,'???'
DB 006H,01,00,0C3H,'???'
DB 010H,01,01,0C4H,'JMP PAGE 6, #'
DB 008H,01,00,0C5H,'SEL R0'
DB 006H,01,01,0C6H,'JZ'
DB 00DH,01,00,0C7H,'MOV A,PSW'
DB 00AH,01,00,0CBH,'DEC R0'
DB 00AH,01,00,0C9H,'DEC R1'
DB 00AH,01,00,0CAH,'DEC R2'
DB 00AH,01,00,0CBH,'DEC R3'
DB 00AH,01,00,0CCH,'DEC R4'
DB 00AH,01,00,0CDH,'DEC R5'
DB 00AH,01,00,0CEH,'DEC R6'
DB 00AH,01,00,0CFH,'DEC R7'
DB 00DH,01,00,0D0H,'XRL A,@R0'
DB 00DH,01,00,0D1H,'XRL A,@R1'
DB 007H,01,01,0D2H,'JB6'
DB 008H,01,01,0D3H,'XRL A, #'
DB 011H,01,01,0D4H,'CALL PAGE 6, #'
DB 008H,01,00,0D5H,'SEL R1'
DB 006H,01,00,0D6H,'???'
DB 00DH,01,00,0D7H,'MOV PSW, A'
DB 00CH,01,00,0DBH,'XRL A,R0'
DB 00CH,01,00,0D9H,'XRL A,R1'
DB 00CH,01,00,0DAH,'XRL A,R2'
DB 00CH,01,00,0DBH,'XRL A,R3'
DB 00CH,01,00,0DCH,'XRL A,R4'
DB 00CH,01,00,0DDH,'XRL A,R5'
DB 00CH,01,00,0DEH,'XRL A,R6'
DB 00CH,01,00,0DFH,'XRL A,R7'
DB 006H,01,00,0E0H,'???'
DB 006H,01,00,0E1H,'???'
DB 006H,01,00,0E2H,'???'
DB 00EH,01,00,0E3H,'MOV @R0, A'
DB 010H,01,01,0E4H,'JMP PAGE 2, #'
DB 008H,01,00,0E5H,'SEL R0'
DB 007H,01,01,0E6H,'JNC'
DB 007H,01,00,0E7H,'RLA'
DB 00DH,01,01,0EBH,'DJNZ R0, #'
DB 00DH,01,01,0E7H,'DJNZ R1, #'
DB 00DH,01,01,0EAH,'DJNZ R2, #'
DB 00DH,01,01,0EBH,'DJNZ R3, #'
DB 00DH,01,01,0ECH,'DJNZ R4, #'
DB 00DH,01,01,0EDH,'DJNZ R5, #'
DB 00DH,01,01,0EEH,'DJNZ R6, #'
DB 00DH,01,01,0EFH,'DJNZ R7, #'
DB 00DH,01,00,0F0H,'MOV A,@R0'
DB 00DH,01,00,0F1H,'MOV A,@R1'
DB 007H,01,01,0F2H,'JB7'
DB 006H,01,00,0F3H,'???'
DB 011H,01,01,0F4H,'CALL PAGE 7, #'
DB 008H,01,00,0F5H,'SEL R1'
DB 006H,01,01,0F6H,'JC'
DB 009H,01,00,0F7H,'RLC A'
DB 00CH,01,00,0FBH,'MOV A,R0'
DB 00CH,01,00,0F9H,'MOV A,R1'
DB 00CH,01,00,0FAH,'MOV A,R2'
DB 00CH,01,00,0FBH,'MOV A,R3'
DB 00CH,01,00,0FCH,'MOV A,R4'
DB 00CH,01,00,0FDH,'MOV A,R5'
DB 00CH,01,00,0FEH,'MOV A,R6'
DB 00CH,01,00,0FFH,'MOV A,R7'

```

23. HISTOGRAM DISPLAY

23.1 INTRODUCTION

The Histogram function calculates statistics on the data in Sample Memory. It is primarily used for studying program execution to improve efficiency. When the data in Sample Memory represents addresses of instructions in a computer program, the Histogram can be used to measure how much time the computer spends executing different parts of the program.

An example of the Histogram Display, which combines menu and display on the same screen, is shown in Exhibit 23-1.

A histogram is the result of a statistical procedure in which items are sorted into different categories according to some characteristic, and then the items in each category are counted.

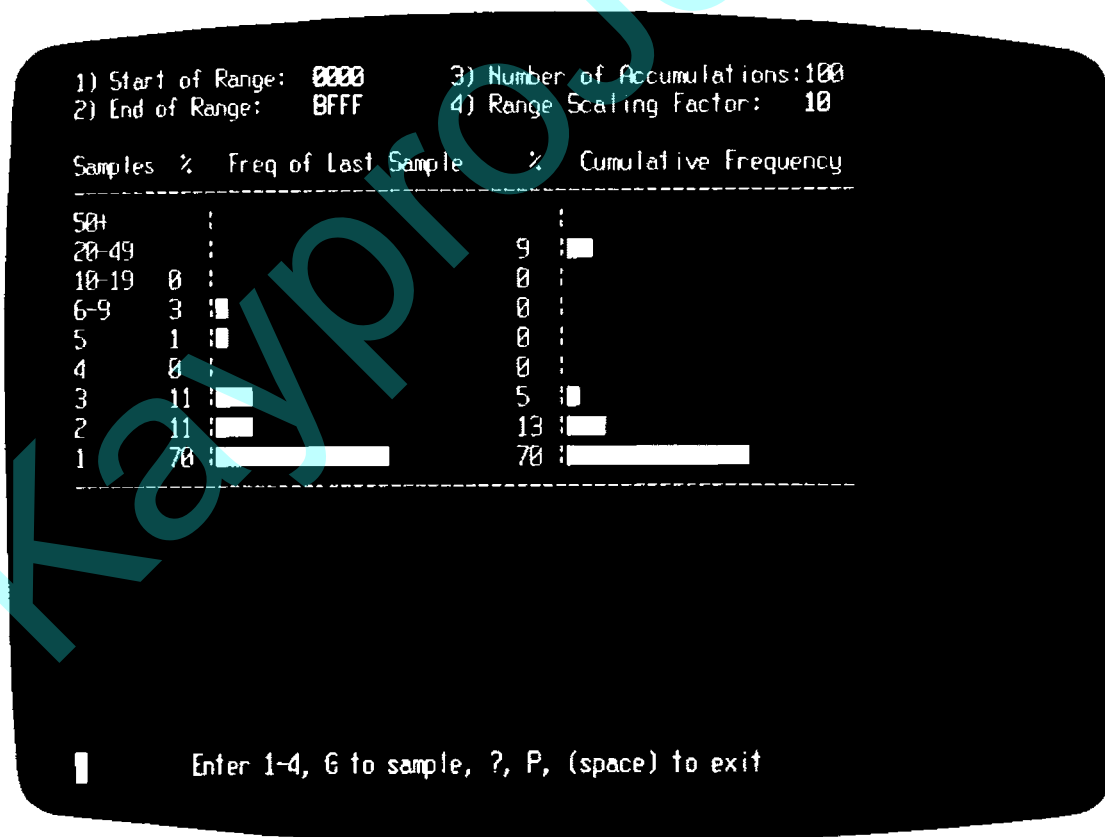


Exhibit 23-1. Histogram Display. Typical values have been entered in Items 2, 3, and 4 to provide an example.

The algorithm that produces the Histogram Display works as follows. It looks through the Sample Memory for sample data falling in the range specified in Items 1 and 2; let us call those "in-range samples." An in-range sample will sometimes appear in a "run" of in-range samples (that is, with other in-range samples before or after it, or both) and sometimes all alone. .

Two questions are of interest here. First, how long are the "runs" of in-range samples - how many samples are there in each run? Second, and more important, how are the samples distributed in the runs of different lengths - how many samples fall in short runs versus long runs? So the histogram algorithm identifies the "runs" of in-range samples, sorts them into categories by length of run, and then counts the number of samples in each category.

Refer now to Exhibit 23-1. The column on the left gives run lengths, that is, "6-9" means runs 6 to 9 samples long. The second column is the percentages of in-range samples that fall in the runs of different lengths. The exhibit shows that 3% of the in-range samples fall in runs 6 to 9 samples long.

Note that the base for the percentage (100%) is the total number of in-run samples in the Sample Memory. Thus the percentages shown in the histogram will always total (approximately) 100%.

This may be applied to computer operation as follows. A microprocessor fetches instructions from memory in a sequential fashion, incrementing its program counter one, two, or three bytes, depending on the length of the instruction. Program loops or branches, however, cause the sequence to change. While a program may have no more than a dozen instructions within a certain address range, if a loop is there, the processor may make thousands of instruction fetches all within in that same address range.

Thus long "runs" of instruction fetches within a certain range of addresses reveal intense activity within that part of the program. By making a number of Histograms Displays with different range settings, you can identify which parts of the program are using the most execution time.

There are three steps to using the Histogram function.

First, attach the probes to the appropriate points in the equipment you are testing. Set up the data collection conditions on the Trigger Menu and (if necessary) the Options Menu.

Second, call up the Histogram Display with the H Command and enter the desired parameters in the menu items - the upper and lower limits of the range in Items 1 and 2; if multiple accumulations for better statistical averaging are required, the desired number of accumulations in Item 3; and if run length categories other than the default values are desired, the Scaling Factor in Item 4.

Third, type "G" to cause data collection. Each repetition of the G Command collects new data.

23.2 HISTOGRAM MENU

As with the other menus, type the item number to put the entry cursor on a menu item. The following paragraphs give more details about the individual menu items on the Histogram Display.

Item 1) Start of Range:

Enter the lower limit for the range in this item. The lower limit must be a number between 0000 and FFFF hexadecimal (0 and 65,535 decimal). The default radix is hexadecimal. The number entered should contain a radix suffix (e.g., D for decimal, O for octal, B for binary) if some value other than hexadecimal is input. Numbers entered in octal will be immediately converted to hexadecimal on the display.

The value entered here also depends on the active channels selected in the Trigger Menu, T Command. Channels that are not active are treated as "don't care" values both in the data sampled and in the numbers specified in Items 1 and 2. For example, if only the lower eight channels are active, and they are connected to a computer address bus, then all address bits except the lower 8 will be "don't cares". This will usually increase the number of samples that will be counted as in-range.

Inactive channels are assigned a binary value of 0 for display in this item. For example, assume that 3333h is entered in this item while Channels 1 and 0 are inactive. The Omni converts 3333h internally to its binary equivalent, "0011 0011 0011 0011". Since Channels 0 and 1, which correspond to the last two bits, are inactive, the last two bits are changed to "00", so the binary number becomes "0011 0011 0011 0000". The hex equivalent, "3330", is then displayed in Item 1. All this is done automatically when you type in "3333".

Item 2) End of Range:

Enter the upper limit for the range in this item. The comments above regarding the number entered in Item 1 also apply here.

Item 3) Number of Accumulations:

The Histogram function can perform repeated accumulations for better statistical accuracy. Each individual histogram (left set of bars in Exhibit 23-1) is generated from the 1000 samples of one data collection cycle. For some applications, 1000 samples may not be enough to give statistically significant averages. With a sufficient number of data collections, however, a good statistical account of the event can be generated on the cumulative histogram (right set of bars). Enter the number of repeated collections desired in this item. If a 0 (zero) is entered in Item 3, the Omni will repeat accumulations until the space bar is pressed.

Item 4) Range Scaling Factor:

Here "range" in the name of Item 4 means "run lengths." Nine categories of run lengths appear to the left of the display. The default categories divide the in-range samples into runs of 1, 2-4, 5-9, 10-19, 20-49, 50-99, 100-199, 200-499, and 500+ samples. For an entry to be made in the 2-4 category, for example, the data collected must have fallen within the range specified via Items 1 and 2 for at least 2 but no more than 4 consecutive samples.

Finer resolution can be obtained by scaling. Scaling by a factor of 10 will then put the top category at 50+ and the shorter periods proportionately narrower. If scaling is desired, enter the scale factor in Item 4.

23.3 DISPLAY CHARACTERISTICS

Features of the statistical data produced by the Histogram function and shown on the display are:

Samples - the categories of run lengths for which statistics are collected: runs of 500+ samples, runs of 200-499 samples, and so on in the default case. The example in Exhibit 23-1 uses a Scaling Factor of 10, yielding run length categories of 50+, 20-49, and so on.

% - the percentage of in-range samples falling in runs of the various length categories. The base for the percentage is the total number of in-range samples, that is, the samples lying in the range given in Items 1 and 2. In the example shown in Exhibit 23-1, 3% of the samples lying within the range 0000H to BFFFH are in runs of 6 to 9 samples; 1% lie within runs 5 samples long; and so on. The first % column expresses the statistics for the most recently collected data.

Freq of Last Sample - histogram prepared based on the data most recently collected by the G Command. The bar length is proportional to the percentage to its left, just defined above.

% - same statistic as that contained in the first % column, except that it expresses statistics accumulated (averaged) over a number of data collections. In order to get enough data to make a statistically significant histogram, it may be necessary to accumulate data over several samplings. The example shows a histogram accumulated during 100 data collections.

Cumulative Frequency - histogram based on statistics accumulated (averaged) over a number of data collections. The bar length is proportional to the percentage just to its left.

23.5 HELP PAGE

A Help Page for this function appears in response to "?H". When viewing the Histogram Display, Help Pages for the individual menu Items 1, 2, etc., may be accessed by typing "?1", "?2", and so on. After viewing a Help Page, press <SPACE> to return to the Histogram Display.

Kaypro Journal

Rev. D

24. SIGNATURE ANALYSIS

24.1 INTRODUCTION

A signature is a checksum calculated from the data stream passing a circuit node. A very powerful troubleshooting technique, signature analysis is used to isolate faults in defective circuit boards. The user compares the signatures at various points on a malfunctioning board to the signatures for a known good board.

The Omni's signature analysis function is controlled by a combined menu and display which appears in response to the S Command. Exhibit 24-1 shows an example of the menu and display.

1) Start on: U9-PIN6	LOW LEVEL	Channel	Sample	Reference
		TEST-POINT-D	80AE <-->	0353
2) End on: U12-PIN9	LOW LEVEL	U36-PIN25	BA27 <-->	29DE
		U36-PIN19	9E2D <-->	B7AE
3) Clock Polarity:	NEG EDGE	J3-PIN23	D8BC <-->	7C5B
4) Clock Qualify:	DONT CARE	U12-PIN3	0D10 <-->	D183
		U41-PIN11	953F <-->	41B8
5) Trig Enable on:	DONT CARE	U43-PIN5-DECODE	2876 <-->	B788
		U6-14--CLOCK(C)	B788	B788
		U9-14--CLOCK(B)	BA10 <-->	25EE
6) Save to file:		U7-9--CLOCK(A)	69D3	69D3
7) Read from file:	S3	U47-PIN16	B788 <-->	2876
8) Read setup file:		TEST-POINT-A	B788	B788
9) Delete signature file:		U4-9-SYNC-DET	BA10 <-->	25EE
Number of Samples:	1012	DATA-INPUT	69D3	69D3

Enter 1-9, G to sample, ?, P, (space) to exit

Exhibit 24-1. Signature Menu (left) and Display (right two columns). Sample signatures that differ from the Reference signatures are marked by a "<-->" symbol and highlighted.

The signature analysis algorithm generates a four digit hexadecimal number. Many manufacturers of digital electronic products now provide signature test points and correct signatures in their service manuals, making signature analysis possible on the service bench as well as the production line.

The Omni can perform signature analysis on up to 14 test points simultaneously. It can collect "reference good" signatures; store them on disk; recall them from disk; and collect test signatures and compare them to the reference signatures.

There are three steps in performing a signature analysis:

First, connect the probes to the equipment to be tested. Connect the Omni's Clock probe lead to a circuit point carrying the clock signal that will be used. When collecting signatures, the Omni uses the D0 line to sense a Start signal and the D1 line to sense an End signal; connect the probe leads to those signals. Finally, collect one or more of the other 14 data lines, D2 through DF, to the circuit nodes at which the signatures are to be taken.

Note that any one, all, or any combination of the 14 lines may be used simultaneously, making thorough testing at multiple test points very easy. (In fact, when used with a bed-of-nails board test fixture, the Omni will perform most of the functions of a large production board test system at a fraction of the cost.)

Second, enter the appropriate parameters on the menu - polarities of the Start and End signals, Clock Polarity, and if desired, Clock Qualify and Trigger Enable conditions. If comparison with Reference signatures saved on disk previously is desired, enter the name of the file in Item 7. (How to put the Reference signatures on the disk is explained below.)

Third, type "G" to collect samples and generate the test signatures, which will appear in a column under "Sample". Any signatures which differ from the corresponding Reference signatures to the right will be highlighted.

Reference signatures are created by collecting signatures from a known good board; saving the signatures to a disk file using Item 6; then recalling the disk file data to the Reference signature memory using Item 7. Details on this and other aspects of using signature analysis are given below.

NOTE: Reference signatures can be saved to disk and recalled only by using Items 6 and 7 on the Signature Menu. The save and recall functions on the File Menu operate only on sample and reference data, which are different from sample and reference signatures. Signature files have extension ".LAS", while data files have extension ".LAD".

24.2 MENU ITEMS

Details about the individual menu items are given in the following paragraphs.

Item 1) Start on:

All signals entering the logic analyzer are ignored until the level specified for the Start level (high or low) is detected on Channel 0. Signature generation begins with the first sample collected after the start condition is satisfied.

Enter a "1" in Item 1 to indicate a high Start level, or a "0" to indicate a low Start level.

Item 2) End on:

Enter a "1" in Item 2 to indicate a high End level, or a "0" to indicate a low End level.

Signature generation continues for all samples collected up to, but not including, the sample during which the end condition is satisfied. If an End signal does not occur within 1000 samples of the Start signal, signatures will be calculated based on the first 1000 samples after the Start signal. Thus if it is important that the signatures be based on a hardware End signal, take care to select an end condition that will occur within less than 1000 samples of the start condition.

Item 3) Clock Polarity:

Signature analysis requires an external clock signal from the equipment under test. Internal clocking is inappropriate for signature and is not allowed. Select the external clock edge that will provide valid data for the type of circuit being tested. For example, if a microprocessor's active low read control line is used as the external clock input, then the positive edge would be used to collect data since the processor data bus is stable on the positive edge. Enter a "1" in Item 3 to indicate clocking on the positive (rising) edge, or a "0" to indicate the negative (falling) edge.

Item 4) Clock Qualify:

Data collected for signature analysis is recorded on the clock edge, but only when the Clock Qualify line is at a specified level. If no qualification is desired so that every clock edge records a sample, then the "don't care" condition should be used. If data collection is to occur when the qualify line is at a high level, enter a "1". Enter a "0" to allow data collection only when the clock qualify line is at a low logic level. Entering "X" makes this item "don't care", which is the default condition. This function increases the flexibility of data collection.

Item 5) Trig Enable on:

The Trigger Qualify line can be used to enable the Start condition, so that data collection begins only when both Channel 0 and the Trigger Qualify line match their specifications. Enter a "1" in Item 5 to achieve trigger enable on a high level. Enter a "0" to achieve trigger enable on a low level. If you do not wish to use trigger enable to qualify Start collection, enter an "X".

Item 6) Save to File:

Signature values for all fourteen channels can be saved on disk for later reference by entering the filename under which they are to be saved in Item 6. Enter a filename of up to eight characters. A drive specification can also be included per the usual operating system convention (e.g., B:FILENAME). The extension ".LAS" is automatically appended to the filename; if a extension is entered, it is ignored.

The setup information used to collect the data is also saved on disk. The Reference signatures are not saved. (They are already on disk, and will remain there.) The saved data can be retrieved by using either Item 7 or 8.

Item 7) Read from file:

Signatures which were saved with Item 6 can be retrieved and placed in Reference Memory for comparison with the newly sampled signatures. Sample signatures that do not correlate with Reference signatures are highlighted. Enter a filename as in Item 6 above. If the file does not exist, a message to that effect will be flashed on the screen.

Item 8) Read setup file:

This item allows retrieval of signatures and set-up information stored on disk. The hardware will then be configured according to this set-up information. This option can be used to repeat a test performed at an earlier time.

Item 9) Delete signature file:

To delete a signature file, enter its name (without the extension) in Item 9, followed by <RETURN>. It will be immediately erased from the disk.

Number of samples:

This parameter on the menu shows the number of samples used in generating the signatures, which is equal to the number of clock cycles between the Start and End signals.

24.3 HELP PAGE

A Help Page for the Signature Analysis function may be called up with "?S". When viewing the Signature Analysis Menu, you can call up individual Help Pages for Item 1, Item 2, etc., with the commands "?1", "?2", etc. After viewing the information, press <SPACE> to return to the Signature Analysis Menu.

KayproJournal

Rev. D

25. PRINTER OUTPUT

25.1 INTRODUCTION

Any of the data displays - such as Waveform, Edge, Dump, Instruction Disassembly, Histogram, Matrix, Signature, etc. - may be sent to a printer for a permanent hardcopy record by using the CTRL-P Command, Printer Output. CTRL-P ("control P") is activated by holding down the <CTRL> key and striking the "P" key. The "P" key can be upper or lower case.

25.2 COMMAND FORMAT

Anytime the prompt cursor appears in the lower left corner of the screen, you can use one of the following formats to print what is shown on the screen:

- CTRL-P Print the information displayed on the screen.
- CTRL-Px Print the information shown on the screen, starting at sample x.
- CTRL-Px,y Print the collected data from sample x to sample y, in the same format in which it was last displayed on the screen.
- CTRL-P? Print all Help Pages on the printer.

The samples x and y may be designated either by the sample numbers, or if Internal Clock is being used so that there is a meaningful time scale, by the sample times.

25.3 EXAMPLE

- CTRL-P 10,50us Print data from sample number 10 through the sample collected 50 microseconds after the trigger. The display mode will be the same as last shown on the video screen.

25.4 CONNECTING THE PRINTER

Either the Parallel Port or Serial Port may be used to drive the printer. Normal output is to the Parallel Port. If you wish to use the Serial Port, use the CP/M program STAT to direct output to the the Serial Port:

```
A0>STAT LST:-TTY:
```

Further information on setting up the ports (baud rate, etc.) for your printer may be found in the user's guide for the computer.

The Omni expects to receive standard "ready" handshaking signals

from a printer when data is sent out. If you use the CTRL-P Command and no printer is connected, the Omni will go into a wait loop, waiting for a nonexistent handshake signal. To recover from this, use the Reset function and start over. Any data in the Sample Memory and your parameter settings will be lost when you use Reset. To avoid this, make sure a printer is connected and operable before you use the CTRL-P Command.

Omnis manufacture before mid-1984 have a single serial port, while units made later have two serial ports, one for a printer and one for data. On the units with one port, the port is configured as a DTE port under the RS232C standard. Serial data is sent out on pin 2 of the connector, and received on pin 3. When used for printing as the LST: port under CP/M, it requires a HI handshaking signal from the printer on pin 5. If your printer does not provide this signal, you can jumper pin 5 to pin 6, where a HI signal is present.

On the units with two serial ports, The data port (labeled "J4 SERIAL DATA I/O") is configured the same way as the single port described in the previous paragraph. It is not accessed as the TTY: port by CP/M, however; your applications software (such as a modem program) will access it directly.

On units with two serial ports, the printer port (labeled "J3 SERIAL PRINTER OUPUT") is the CP/M TTY: port. It is configured as a DCE port under the RS232C standard. Data is sent out on pin 3 and received on pin 2. Pin 20 is used for handshaking; it must be driven HI for data to be sent out when this port is made the LST: port using the STAT command. There is no handy HI signal source present on the connector.

In printing waveforms, the Printer Output function uses the underscore "_" to represent a low, the tilde "~" to represent a high, the slash "/" to represent a leading edge, and the backslash "\" to represent a trailing edge. Many dot matrix printers allow downloading a custom character set which gives a better graphic representation of waveforms. The character downloading may be performed by a small program which is run before loading the Logic Analyzer Program.

Exhibit 25-1 shows an example of such a program, and Exhibit 25-2 shows the resulting waveform printout.

25.5 HELP PAGE

A Help Page for the CTRL-P Command may be accessed by typing "?CTRL-P".

```

; THIS PROGRAM CREATES A DOWNLOAD CHARACTER SET FOR
; PRINTING THE OMNI II TIMING TRACES ON A STAR
; gemini-10X PRINTER. ALL CHARACTERS ARE STANDARD
; EXCEPT:
;
;      (/) WHICH IS CHANGED TO A VERTICAL LEADING
;      EDGE WITH A FLAT TOP.
;
;      (\) WHICH IS CHANGED TO A VERTICAL TRAILING
;      EDGE WITH A FLAT BOTTOM.
;
;      (~) WHICH IS CHANGED TO A FLAT TOP.
;
; VERTICAL ALIGNMENT IS ALSO ASSURED BY SETTING UNI-
; DIRECTIONAL PRINTING. NORMAL PRINTER OPERATION MAY
; BE RESTORED BY TURNING IT OFF AND THEN ON AGAIN.

```

PROGRAM EQUATES

```

0005 =   BDOS      EQU      05H      ;DOS ENTRY VECTOR
0005 =   LSTFUNC   EQU      05H      ;DOS LIST FUNCTION
001B =   ESC       EQU      1BH      ;ASCII FOR ESCAPE
00FF =   TERM     EQU      OFFH     ;STRING TERMINATOR
0100 =                   ORG      100H

; THIS ROUTING READS AND TRANSMITS THE CONTROL
; SEQUENCES LOCATED AT "STRING".
0100 211501   DNLDCHR LXI  H,STRING ;GET POINTER
0103 7E       DNLD2  MOV  A,M      ;GET A CHAR
0104 FEFF    CPI    TERM          ;TERMINATOR?
0106 CA0000  JZ     0             ;YES, RETURN TO CP/M
0109 E5     PUSH  H              ;NO, SAVE POINTER
010A 5F     MOV  E,A            ;CHAR TO E REG
010B OE05   MVI  C,LSTFUNC      ;AND OUT TO PRINTER
010D CD0500 CALL  BDOS
0110 E1     POP   H              ;RESTORE POINTER
0111 23     INX  H              ;BUMP POINTER
0112 C30301 JMP  DNLD2          ;AND GET NEXT CHAR

0115 1B2A00   STRING DB   ESC,'*',0 ;COPIES STD CHAR'S TO
;DOWNLOAD RAM.
0118 1B2A01   DB   ESC,'*',1 ;CHANGES /
011B 2F007F0001 DB   2FH,0,7FH,0,1,0,1,0,1,0,1
0126 1B2A01   DB   ESC,'*',1 ;CHANGES \
0129 5C017F0040 DB   5CH,1,7FH,0,40H,0,40H,0,40H,0,40H
0134 1B2A01   DB   ESC,'*',1 ;CHANGES ~
0137 7E00010001 DB   7EH,0,1,0,1,0,1,0,1,0,1
0142 1B2401   DB   ESC,'$',1 ;ACTIVATES DOWNLOAD SET
0145 1B5501   DB   ESC,'U',1 ;SETS UNI-DIRECTIONAL
;PRINT
0148 FF     DB   TERM
0149                END

```

Exhibit 25-1. Hubert Evinger of Advanced Computer Concepts, Inc., Costa Mesa, California wrote this CP/M program for downloading special waveform characters to a STAR gemini-10X printer.

26. THEORY OF OPERATION

26.1 INTRODUCTION

What is a logic analyzer?

A logic analyzer is an instrument for collecting and displaying digital data. Used primarily for testing digital equipment, it has input probes that may be connected to integrated circuit pins inside the equipment under test.

A logic analyzer records the logic levels on many lines, over a period of time, and then displays the recorded patterns. By examining the collected data, you can trace the operation of the digital circuit.

The logic levels are sampled in step with a clock signal. The clock signal either may be generated inside the analyzer (Internal Clock), or may be taken from the equipment under test (External Clock). Each sampling stores one data word in the logic analyzer's Sample Memory. The analyzer continuously collects data in memory until a trigger event, which may be either recognition of a specific word in the data stream or an external event, causes it to stop.

Like an oscilloscope, a logic analyzer collects data corresponding to voltage versus time and displays it as "traces". Two features make the logic analyzer a very powerful tool:

A) It can collect data on many lines at once; in the case of the Omni, on 16 lines, or, with the the 32 Channel Adapter, on 32 lines. Observing the bit stream on a single line at one time, as with an oscilloscope, is of little value, since the bit pattern is meaningful only in reference to the simultaneous bit patterns on other lines.

B) The logic analyzer collects data prior to the trigger event, again unlike an oscilloscope, which starts the trace after the trigger event. When a digital circuit goes awry, the cause is usually found in what happened beforehand, not afterwards.

The logic analyzer has two limitations compared to an oscilloscope - it records voltage as only "high" or "low" (binary 1 or 0), losing the details of waveform shape. Also, it records the logic level only at the clock transitions, thus limiting the time scale resolution to the minimum clock period that the logic analyzer can handle. (This disadvantage is partially remedied by the inclusion of glitch collection capability.) The Omni will accept a clock rate of up to 20 MHz, yielding 50 nanoseconds resolution. Also, there is a trade-off between resolution and length (in time) of the trace; since the Omni can store only about 1000 samples, at the finest time resolution it can store only 50 nanoseconds x 1000 = 50 microseconds of trace. In practice, this limitation proves to be of little hindrance and 1000 samples are quite adequate.

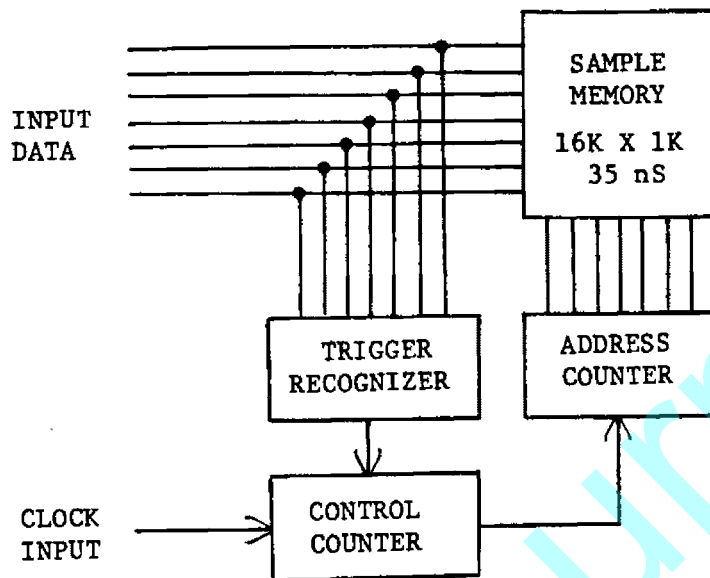


Exhibit 26-1. Diagram of the logic analyzer. The Input Data is picked up by the analyzer probes. The Clock Input can be either an External Clock signal picked up by the probes, or the analyzer's Internal Clock.

26.2 HOW IT WORKS

The heart of the logic analyzer is the Sample Memory (see Exhibit 26-1). As the Clock Input provides clock pulses, the Sample Memory stores samples, one sample for each clock pulse. The clock pulses also step the Address Counter, so that samples are stored in successive addresses in the Sample Memory.

The Sample Memory is 16 bits wide and holds 1024 words, that is, it has 1024 addresses, from 0 through 1023. When the Address Counter reaches 1023, it "rolls over" and stores the next sample at Address 0. Thus old data is continually being overwritten as the analyzer collects new data.

The Trigger Recognizer is also connected to the input data stream, and will have been set (via the Trigger Menu) to detect some combination of bits (the trigger word) in the input data. When the Recognizer detects the trigger word, it initiates the trigger sequence.

The trigger sequence consists of two steps. First, the analyzer continues to collect a certain number of additional samples. The Control Counter manages this, and the purpose is to provide samples in the stored trace after the trigger event, as well as before. (The

number of samples collected beyond the trigger event is entered as the Trigger Point on the Trigger Menu.)

As the second step of the trigger sequence, the analyzer displays the collected samples. The software automatically formats the display according to the parameters entered in the Trigger Menu, which usually call for the trigger event to be labeled Sample 0 and displayed in the center of the screen. The Omni does not display all of the 1024 samples; because of timing uncertainties in the collection process, a few samples at the ends of the trace may be invalid and the Omni excludes them from display.

26.3 TIMING ANALYZERS AND STATE ANALYZERS

Early logic analyzers were one of two kinds, either state analyzer or timing analyzer. The state analyzer was clocked by some cyclical event in a computer, and recorded the "state" (combination of logic levels) at some set of circuit points. It was used for tracing the operation of a computer circuit as it moved step-by-step through its cycle.

When connected to the address bus, and connected to use a read or write control pulse as its clock signal, the state analyzer would trace the sequence of memory reads and writes, thereby tracing program execution. The state analyzer's output was typically displayed as a list of binary words expressed in 1's and 0's.

The state analyzer, while showing the correct sequence of states, does not furnish the data against an accurate time scale unless the clock signal has a uniform and known period.

The timing analyzer, on the other hand, had its own internal free-running clock, and capture data without regard to synchronization with the circuit being observed. The data was shown in a format similar to oscilloscope waveforms, which the timing analyzer was expected to mimic, with the added benefit of multiple traces and before-the-trigger data capture.

The timing analyzer does not show exactly the transition times of the signals it is trying to measure, since the transitions that appear are those of its own clock. Using a 50 nanosecond clock period, for example, the timing analyzer shows a signal transition 0 to 50 nanoseconds after it actually occurs, depending on when the analyzer's clock edge transition occurred compared to the signal being measured.

In order to achieve a reasonably accurate representation of the measured signal, the timing analyzer clock has to be several times faster than the frequency of the events being observed. A popular rule of thumb calls for the timing analyzer's clock frequency to be four to five times higher than the fastest frequency to be observed.

High speed is more important to a timing analyzer than to a state analyzer. A state analyzer need only be as fast as the system clock of whatever it is measuring.

The Omni has both Internal Clock and External Clock modes, allowing it to serve as either a timing or state analyzer. Its 20 MHz clock rate is fast enough to make it quite serviceable as a timing analyzer for microprocessor based systems. This flexibility makes the Omni very easy to use. Furthermore, regardless of how the data was collected, using either internal clock (timing analyzer) or external clock (state analyzer), the data can be displayed in either timing diagram format or state diagram format. Once you have collected the data, you can display it in several formats until you find the one most revealing. Generally speaking, a timing diagram is most useful for studying hardware operation, while a state display is most appropriate for tracing software execution.

The Omni also has a Trigger Out signal which may be used to trigger an oscilloscope for high-resolution examination of waveforms. This enables you to see the data signals in detail - waveform shape, multiple glitches, actual logic levels, and so on. The resolution, which is now determined by the bandwidth of the oscilloscope, can be as fine as 1.5 nanoseconds with a 200 MHz scope.

The Omni's triggering capability allows the oscilloscope to observe events that are associated only with a certain data word, or with the presence of glitches, or with a combination of both.

See Section 7 for further information on using the Trigger Out signal.

26.4 SOURCES OF ERROR

To summarize, the logic analyzer is subject to the following limitations:

The square waveforms appearing in the Waveform and Edge Displays do not represent the actual waveshapes of the signals being recorded. Regardless of the actual waveforms, the input levels are recorded as only HI or LO levels.

A transition in the input is not recorded until the time the next sample is taken. Thus the transitions displayed correspond to the time of sampling, not the transition points in the input waveforms.

Signal activity between sampling points is not recorded, with the following exception. Transitions between sampling points are recorded as glitches on the lower four channels, and will be displayed if glitch display is activated.

Another possible source of error is loading by the analyzer inputs on the circuit under test. This can be very significant with some types of analyzers which use long ribbon cables (over 6 inches) and unbuffered TTL or LS TTL chips for the input. The Omni series analyzers avoid this by using high impedance (1 megohm) buffered probes with 6-inch probe leads, which hold the capacitance to a few picofarads.

Rev. D

27. APPLICATIONS

EXAMPLE 1. A CRT controller that was not putting out any output signal or responding to any input.

"First of all, I checked to see if the clock was running and which lines had signals on them and which were dead.

"I put one of the 8 leads of one probe on the controller clock line and the rest at various places in the circuit. The Trigger Menu's "logic probe" display showed activity on the clock and other lines. I then used the Omni's default sampling conditions - Internal Clock, 50 nanoseconds Sample Rate - and took a sample.

"Looking at the Waveform Displays, I saw that the controller's clock was operating properly. Some of the other lines had activity on them and others did not. Moving the probes around and taking repeated samples, I hunted to find out where the signals were getting stopped. One 74LS138 address decoder had lots of activity on the address and enable pins, but all the output pins remained high. (The 74LS138 generates an active low output on one pin when it is enabled.) Comparing the waveforms for the address and enable inputs, the chip was enabled for address combination 5, which according to the data book would cause a low output on pin 10 - and there was not. Obviously, either the chip was bad, or a short was pulling the output high.

"I replaced the chip, and then the unit worked.

"Total cost - 40 cents in parts and 10 minutes."

Here, the technician was using the Omni to observe activity on the signal lines. While a logic probe can identify active signals, it does not provide any clue to the time relationships of the signals, as was the key here. No sophisticated trigger settings were needed. The Omni's ability to display signals on many lines simultaneously isolated a bad chip quickly.

EXAMPLE 2. A microcomputer displays its turn-on message properly but does not respond to the keyboard.

"I hooked up the Omni's 16 data probes to the address bus to see if the Z80 was reading addresses. I used the system /MEMR (memory read) signal as the clock. The Clock Qualify probe went on /M1 (pin 27 on the Z80) to collect only opcode fetch addresses. I entered all 1's for the Trigger Event. I pressed 'G' (for 'Go and Collect Sample'), let it run for a second, then manually triggered it by hitting the space bar.

"I used 'D -500' to display the captured data in hex.

"Paging through the Dump Display, it was obvious that the Z80 was looping over and over through about 20 bytes of PROM code.

"One of the addresses 2323H. I moved the cursor to 2323H on the display, pressed the '=' key to enter it (2323H) as the Trigger Event. Then when I ran it again, I would see in the trace how it got to 2323H.

"Then I pushed down the Reset button for the microcomputer, and while holding the button down, typed 'G' on the Omni. The Omni started collecting. I released the Reset button. The Omni stopped collecting and went back to the Dump Display with the cursor on 2323.

"Looking at the display, I saw that it was executing PROM code around 2080H just before making a jump to 231CH. Studying the listing of the assembly language code I had written for the ROM, I saw that there wasn't supposed to be a jump like that around 2080H. Using the clue provided by the Omni, I checked the PROM - sure enough, it had one bad bit.

"Without the Omni, I could have spent hours looking for shorted address lines in the system or studying the code listing looking for errors. I wouldn't even have been able to tell whether I had a hardware fault or a software bug without hours of work. This only took me about 40 minutes, and most of that time was spent getting my tools together and taking the cover off the microcomputer."

Rev. D

28. ADVANCED APPLICATIONS

28.1 EXTENDING THE TRIGGER WORD

Some applications may require triggering on more than 17 bits (16 bits on the data lines plus 1 on the Trigger Qualifier allows an effective 17 bit trigger word). Or, you may want to trigger on one 16 bit combination, such as a microprocessor address, while recording some other data, such as 8 bits on the microprocessor's data bus.

With the Omni's External Trigger capability, you can trigger on a word of any length by using some simple external circuitry to generate a trigger pulse. Exhibit 28-1 on the next page shows a circuit that may be used to trigger on a word of up to 64 bits.

The trigger word is identified by 8-bit comparators (TI 74LS682). For a 64-bit trigger word, eight such comparators are required with their outputs ANDED. The schematic shows only one comparator; the circuit for the others is identical.

The comparators' Q inputs contain internal pull-up resistors, so no external resistors are needed. Each switch is used to set one bit in the trigger word. Switch closed is a "0", switch open is a "1". For a "don't care" ("X") bit, tie the P input of the LS682 high (+5V) and set the corresponding switch open. The comparator will see a high on both inputs, satisfying the trigger condition if all the other inputs match.

You can use fewer than eight 74LS682's for fewer inputs. Tie the unused inputs of the LS30 high (+5V).

28.2 COLLECTING DATA WIDER THAN 16 BITS

Using the Trigger Pulse Generator will also allow you to collect data wider than the Omni's 16-bit word by making more than one collection pass. With the Trigger Pulse Generator recognizing the trigger word, you can move the data probes around to collect multiple sets of data.

For example, assume that you want to collect data on 32 lines. Connect the Omni data probes to 16 lines, collect the data, reconnect the probes to the second set of 16 lines, and collect data again. The data from the two passes may be combined for 32 bits total.

Printer output is especially useful here. The data from each pass can be printed on paper, then the two sheets spliced together for a 32-bit "display". Given enough time, patience, and cellophane tape, you can get data displays of any length word.

28.3 ADDED DELAYS AND LOADING

The delay from the P inputs of the 74LS682 to the output is specified as 25 nanoseconds maximum. This delay adds a 25 nanosecond

hold time requirement for the data signals; normally the hold time required for the data signals is zero. If this proves critical to your application, it may be necessary to put buffers on the inputs to delay the data signals by a matched amount.

The comparator inputs add one TTL load to the circuit to which they are connected. This will not be a problem for equipment with adequate design margins, but it should be considered, particularly if other loads are applied to the same circuit points during the testing.

Rev. 5-8-85

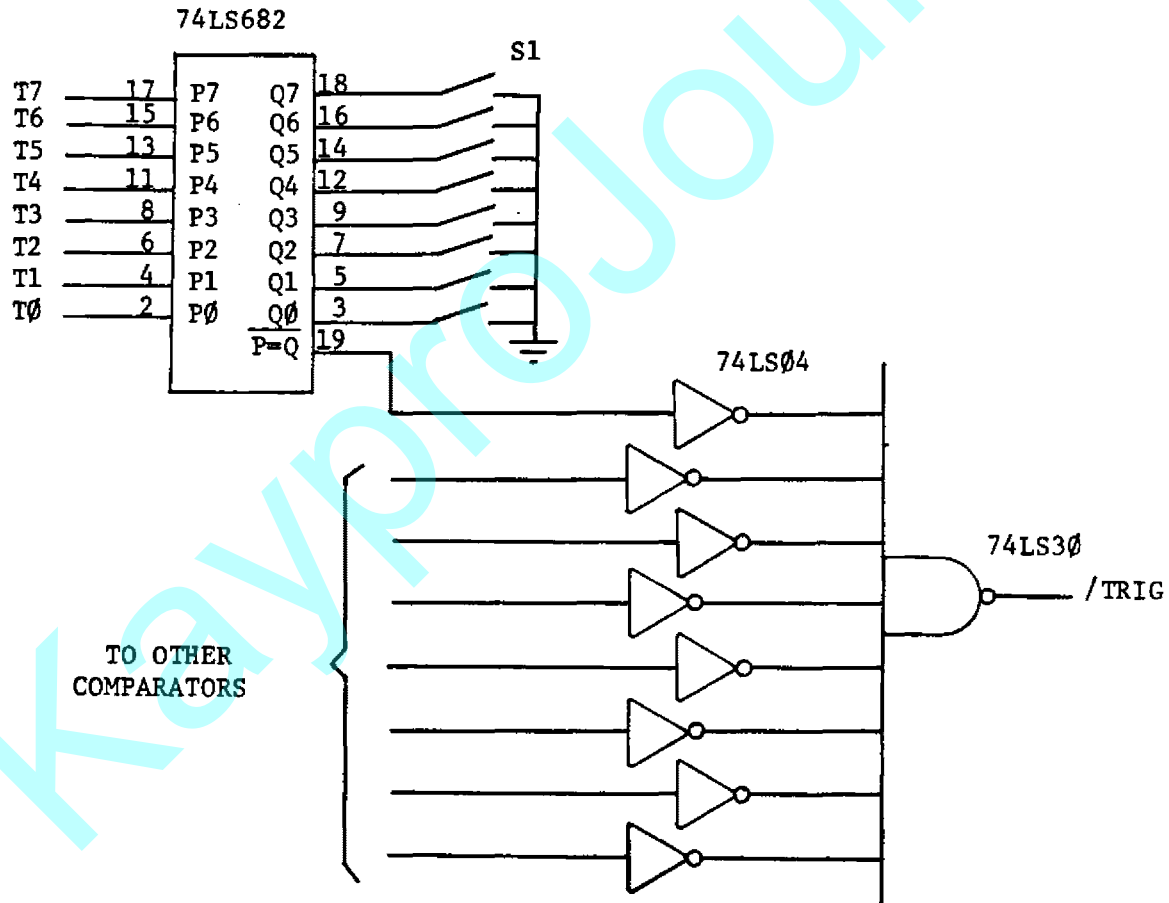


Exhibit 28-1. Trigger pulse generator. When the trigger word appears at the inputs, a /TRIG signal is generated that may be used to drive the Omni's External Trigger probe line.

Rev. D

29. 32 CHANNEL ADAPTER

29.1 INTRODUCTION

The 32 Channel Adapter is an accessory for the Omni that extends its data collection capacity to 32 channels total. The added 16 channels are called Bank 1, Channels AF-A0. The original 16 channels are considered Bank 0, and retain their original designations, DF-D0. Four connectors on the Adapter accept four standard Omni buffered probes (TTL or CMOS type), each of which handles 8 data channels.

The Adapter mounts externally, on the right hand side of the Omni. See Exhibit 29-1. Two cables from the Adapter plug into the probe connectors below the disk drives.

The control lines associated with the original 16 channels (Clock, Clock Qualify, Trigger, and Trigger Qualify) remain identical.

The 32 Channel Mode also provides three clock inputs, called External Clock, External Clock 2, and Multiplexer Clock. The latter is useful for collecting data, particularly for Instruction Disassembly, from microprocessors such as the 8085 that use a multiplexed data and address bus.

Most of the Omni's functions are the same with the 32 Channel Adapter, except extended to the additional channels. This section describes the differences.

When the Adapter is installed, the Omni has two basic modes of operation, 32 Channel Mode and 16 Channel Mode. In 16 Channel Mode, the operation is nearly identical to that without the Adapter. 16 Channel Mode is retained to provide some functions that are not available in 32 Channel Mode.

When using 32 Channel Mode, the maximum data collection rate is 10 MHz (100 nanosecond resolution) and the trace depth is 500 samples. The maximum trigger word width remains 16 bits (17 bits including the Trigger Qualify input). 32 Channel Mode is designed solely for use with an external clock; it will not work with the Internal Clock. Also, no glitch collection capability is available. Glitch collection and Internal Clock are available in 16 Channel Mode.

29.2 INSTALLING THE 32 CHANNEL ADAPTER

The 32 Channel Adapter may be installed on the Omni with ordinary hand tools. Follow these six steps:

- a. Loosen the lower two Phillips-head screws that hold the hood on the right side. Be careful not to scratch the finish.



Exhibit 29-1. The 32 Channel Adapter is a slim box that attaches to the right side of the Omni.


b. Slide one flange of the metal right-angle strip under the hood.

c. Hook the fingers at the top of the 32 Channel Adapter into the vent holes in the hood, so the Adapter hangs from the fingers and the mounting holes on its lower edge line up with the holes in the right-angle strip.

d. Insert the screws through the angle strip into the Adapter, and while pressing the adapter against the side of the Omni, tighten them securely.

e. Tighten the screws holding the hood to the Omni on the right side.

f. Plug the two ribbon cable connectors from the Adapter into the connectors on the front of the Omni. The shorter ribbon cable goes to the nearer connector.

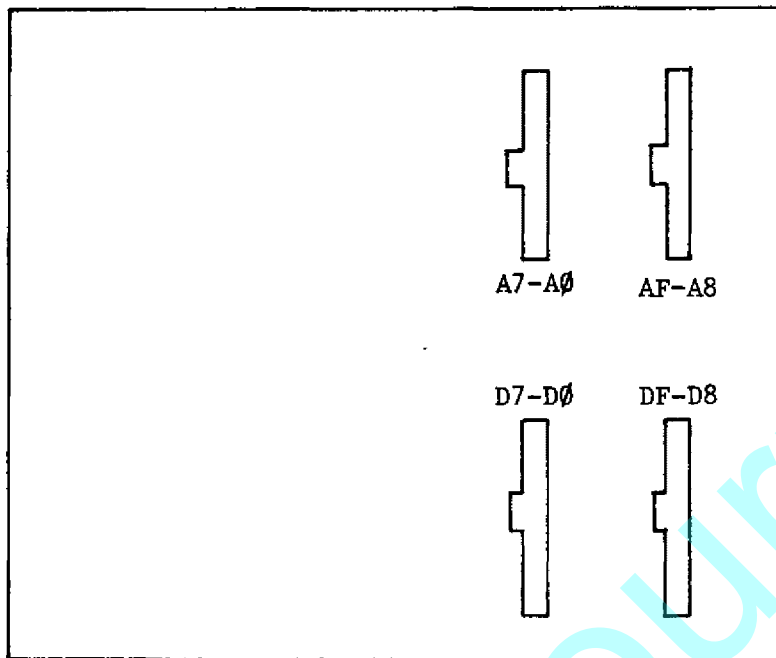

<u>Probe</u>	<u>Data</u>	<u>C Input Line</u>	<u>T Input Line</u>
1	D7-D0	Ext Clock	Ext Trig
2	DF-D8	Clock Qual	Trig Qual
3	A7-A0	Ext Clock 2	Not Used
4	AF-A8	Mux Clock	Not Used

Exhibit 29-2. The buffered probes plug into four connectors on the side of the 32 Channel Adapter.

Exhibit 29-2 shows the order in which the buffered probes are plugged into the 32 Channel Adapter.

29.3 LOGIC ANALYZER PROGRAM

A special version of the Logic Analyzer Program called LA32.COM is used to operate the Omni with the 32 Channel Adapter. The special program also has a 16 channel mode, so that you can use the Omni as before.

Five of the menus and displays have been modified to accommodate 32 channel operation: the Trigger Menu, Options Menu, Dump Display, Instruction Disassembly, and the Locate Function. The shift between 32 Channel Mode and 16 Channel Mode is controlled by the Trigger Menu.

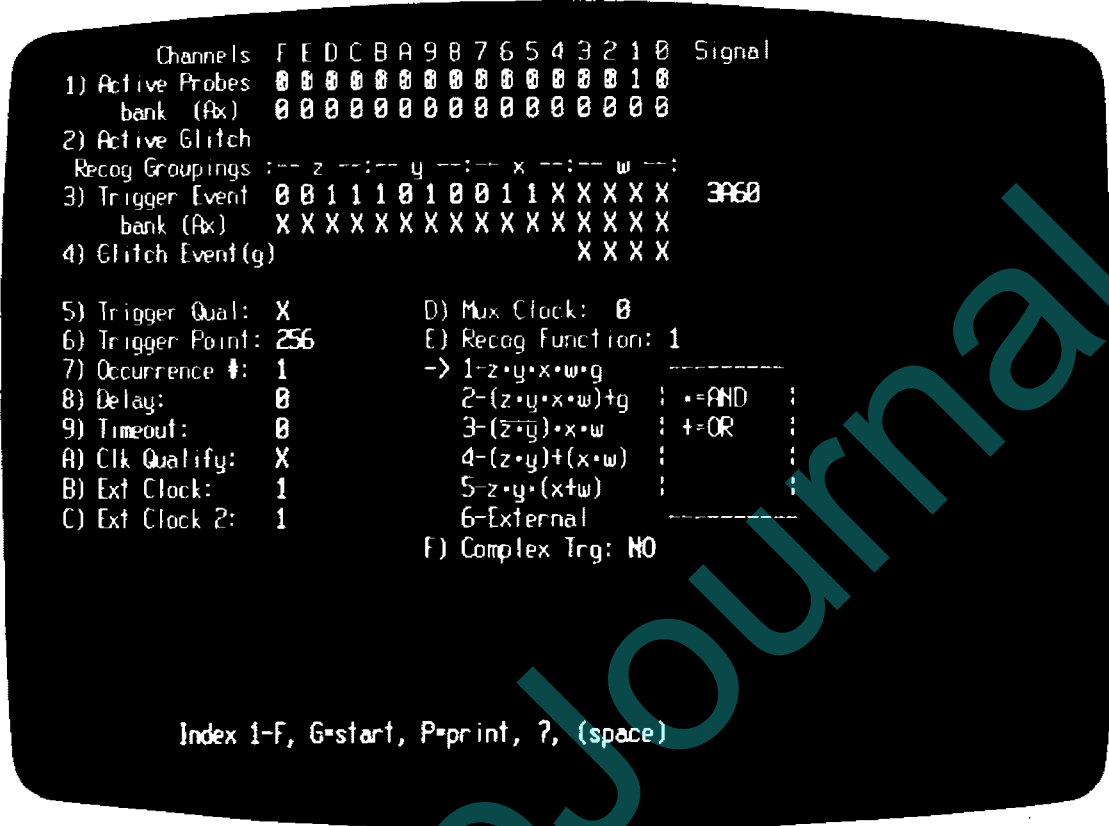


Exhibit 29-3. Trigger Menu used with the 32 Channel Adapter. The Omni is in 32 Channel Mode here. When it is in 16 Channel Mode, Channels AF-A0 are all blank in Item 1. Also, Items C and D are different; Item C is used to enter the Sample Rate and Item C the Recognition Mode, the same as when the Adapter is not used.

29.4 TRIGGER MENU

Exhibit 29-3 shows an example of the 32 Channel Trigger Menu. It has several major differences from the standard Trigger Menu. Details about the changed menu items are given below. Item 1 controls the shift between modes.

Two menu items change when the mode is changed. In 16 Channel Mode, Item C becomes Sample Rate and Item D becomes Recognition Mode - the same as in normal 16 channel operation without the Adapter.

Item 1) Active Probes

This item has been expanded to apply to 32 channels. The channels are divided into Bank 0, DF-D0 (upper row), and Bank 1, AF-A0 (lower row).

To make a given channel active, enter a 1 in its bit position; to make it inactive, enter an X. Active channels are shown by a 1 or 0,

and inactive changes are represent by a blank space. Use the cursor arrow keys to move the cursor from one channel position to another, or keys F,E,...2 may be used for direct cursor positioning.

32 Channel Mode is in effect whenever there are any channels active in Bank 1 (AF-A0). The Omni switches to 16 Channel Mode automatically when no channels are active in Bank 1. The default mode at turn-on is 32 Channel Mode, as shown in Exhibit 29-3.

Only the standard sixteen channels, DF-D0, have the logic probe feature, that is, the ability to show the instantaneous logic state of the probes.

Item 3) Trigger Event

This item is likewise divided into two banks, DF-D0 (upper row) and AF-A0 (lower row). A trigger word may be entered in either bank, but not both at the same time. Only one bank at a time can be active, which means a trigger word may be recognized in either the DF-D0 Channels or the AF-A0, but not both. Accessing a bank makes it active, and the other bank is automatically made inactive - all X's are displayed.

A trigger word formerly displayed in the inactive bank is saved internally. Accessing that bank will again cause the trigger word to be displayed.

Item B) Ext Clock

In 32 Channel Mode, there is no Internal Clock and an External Clock is required. Each of the three clocks, External Clock, External Clock 2, and Multiplexer Clock, is controlled by a menu item. The two External Clock inputs are OR'd together within the Omni, and they act internally as a single clock which simultaneously samples all 32 channels.

The External Clock input line is on Probe 1.

Enter 1 in this item to select the rising edge of the clock pulse as the active edge, or 0 to select the falling edge. While the 16 Channel Mode allows you to enter X to make the External Clock inactive, in the 32 Channel Mode this item will not accept an X. If Probe 1 is disconnected, the External Clock is automatically made inactive. To make it inactive with the probe connected, enter a 1 and leave the probe lead floating (high).

Item C) Ext Clock 2

External Clock 2 is a second external clock input line. It is on Probe 3. The comments above about Item B apply to this item as well.

Item D) Mux Clock

The Multiplexer Clock function is used to demultiplex internally signals taken from a multiplexed source. The Multiplexer Clock signal is picked up by the clock input line on Probe 4.

When the multiplexer function is active, the 8 data bits sensed by Channels DF-D8 (Probe 2) are sampled on the active edge of the Multiplexer Clock signal, and transferred to a latch. The next external clock signal (from External Clock or External Clock 2) will cause the data to be collected from the latch into Channels A7-A0 (normally collected by Probe 3).

Enter 1 in this item to select the rising edge of the clock signal as the active edge, 0 for the falling edge. Enter X to deactivate the Multiplexer Clock function altogether. X is the default entry.

This function is very useful for collecting data from systems which use a multiplexed data bus, such as the 8085 microprocessor. An example of such an application appears at the end of this section.

Item F) Complex Trigger

The Complex Trigger function provides multilevel (sequential) triggering capability. This item is used to activate the Z Menu, which controls it. Merely accessing this item toggles the entry from No to Yes, or vice-versa.

29.5 OPTIONS MENU

The Options Menu has been modified to accommodate the extra sixteen channels. In particular, Items 1 and 2 allow separate specification of the number base in which data is displayed for each of the two banks.

Item 1) Bank 0 (Dx) signals

This item specifies the number base in which the data collected on Channels DF-D0 will be displayed in the Dump Display and other displays that show the data in numeric form. The default choice is hexadecimal. Enter B for binary, D for decimal, U for unsigned decimal, or O for octal.

Item 2) Bank 1 (Ax) signals

Item 2 specifies the number base for Channels AF-A0, similarly to Item 1 for Channels DF-D0.

Item 3) Probe bank used for waveforms

The Waveform Display only shows sixteen channels at a time. Use this item to select which bank will be displayed, the D(x) bank or the A(x) bank. Accessing Item 3 toggles the selection from D(x) to A(x), or vice-versa. Choice of the bank displayed is independent of the bank containing the trigger word; you can trigger on the bank you are not viewing.

29.6 DUMP DISPLAY

Operation of the Dump Display is the same as with the standard version, except that a full 32 bit word is collected and displayed.

Sample	Addr	D0-D7	ctrl	bits	Mnemonic	D8-DF	Bytes
	141	01111111		00111111	ANI	3F	
	143	01111111		00111111 00111111	LXI	H, A082	
	146	01111111		00111111 00111111	LXI	D, 0E00	
	149	01111111		00111111	CPI	04	
	151	01111111		00111111 00111111	JC	5019	
->	154	01111111		00111111	CPI	02	
	156	01111111		00111111	JZ	66	
	158	01111111		00111111 00111111	LDA	9082 00	
	162	01111111			MOV	D, A	
	163	01111111		00111111 00111111	LDA	F482 00	
	167	01111111			ANA	A	
	168	01111111		00111111 00111111	JZ	6F19	
	171	01111111			LDAX	B 03	
	173	01111111		00111111	ANI	E3	
	175	01111111			ORA	D	
	176	01111111			STAX	B	
	177	01111111			PUSH	H	
	178	01111111		00111111 00111111	LXI	H, 7682	
	181	01111111			MOV	E, M 05	
	183	01111111			INR	M 05	
	185	01111111		00111111	MVI	D, 00	
	187	01111111			POP	H A0 82	

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,sp

Exhibit 29-4. Format of display when Instruction Disassembly is used with the 32 Channel Adapter.

This is revealed by the fact that eight hexadecimal digits are highlighted by the cursor, representing the 32 bit word.

29.7 INSTRUCTION DISASSEMBLY

Instruction Disassembly functions the same as in the standard version, except that it is now possible to view 16 channels of address in addition to the 8 channels of data and the control lines. Use Channels AF-A0 for up to 16 address lines, and Channels DF-D8 for the 8 data lines. Two or three of the channels in the remaining group, D7-D0, should be used for the control signals.

Refer to Section 17 of the Omni Operating Manual for details on using the Instruction Disassembly function with various microprocessors. Exhibit 29-4 shows an example of the Instruction Disassembly display provided when the 32 Channel Adapter is used. The full 16-bit address is displayed, as well as the disassembled instructions from the address bus.

29.8 LOCATE FUNCTION

The Locate Menu has been modified to accept 32 bit words as the search keys. In other respects, operation is identical.

29.9 EXAMPLE

The Intel 8085 is an example of a microprocessor for which it is desirable to collect more than 16 channels of data, and demultiplexing is required.

The 8085 uses an 8-bit data bus and a 16-bit address. The upper 8 address bits appear on their own pins, A15-A8. However, both data and the lower 8 address bits are multiplexed on one set of pins, AD7-AD0. The 8085's multiplexing clock signal is called ALE, Address Latch Enable.

In the first part of a memory read cycle, the CPU places the lower 8 address bits on pins AD7-AD0. In 8085 systems, ALE is used to strobe the bits into an address latch. The output of the latch drives the corresponding memory address lines, usually called A7-A0.

In the next part of the cycle, the data bits stored at address A15-A8 are read from memory. The read strobe, /RD, causes the memory to place the data bits on the bus pins, AD7-AD0. (/RD is usually shown in data books as RD. The overbar means the signal is negative-active.)

Connect Probe 2 (Omni Channels DF-D8) to 8085 pins AD7-AD0, and the Multiplexer Clock input lead (Probe 4) to ALE. The address is valid on the falling edge of ALE, so enter 0 in Trigger Menu Item D, Multiplexer Clock.

Connect Probe 4 (Omni Channels AF-A8) to 8085 pins A15-A8. Connect the Omni's External Clock input lead (Probe 1) to the 8085's /RD (read) signal. Data is valid on the rising edge of /RD, so enter 1 in Item B, External Clock. External Clock 2 will not be used, so leave its input probe lead floating (Probe 3) and enter 1 in Trigger Menu Item C, External Clock 2.

When data is collected, the Omni's internal demultiplexing will transfer the lower 8 address bits to Channels A7-A0. The 8085 read strobe will clock the upper 8 address bits into Channels AF-A8. The bits from the 8085 data bus will be collected in Channels DF-D8. The Instruction Disassembly function may then be used to display the collected information in disassembled form.

Rev. D

30. PATTERN GENERATOR

The Pattern Generator is a new accessory for the Omni which has not yet been released. It will be controlled by a menu (accessed by the P Command) in the logic analyzer program, allowing you to use the logic analyzer and Pattern Generator together as an integrated system.

When the Pattern Generator becomes available, a chapter describing its operation will be provided to replace this page.

Rev. D

Appendix A. QUICK START

If you are like most of us, you will want to turn on the Omni and make it do something right away. In this section we will walk you through the Omni's basic functions and displays in about half an hour. The advanced functions take about another hour.

The Omni's computer-based design makes it very easy to learn to use. By the time you are done, you will know most of what you need to know to use the Omni effectively.

I. BASIC FUNCTIONS

A.1 GETTING SET UP

Place the Omni flat on your table. Unfasten the clamps on the right and left sides that hold on the front cover/keyboard, and pull it off. Connect the telephone-type coil cord between the keyboard (rear edge) and the main unit rear panel (near the top). If the rear panel has more than one telephone-type connector, use the one marked "KEYBOARD." Lift the main unit and lower the stand on the underside so that the screen is up and easily visible. Plug the connectors for the probes into the two ribbon-cable connectors below Drive B.

Open the doors of both floppy disk drives. Some types of drives use a pushbutton or lever to latch in the disk rather than a door. Whichever type you have, unlatch the mechanism and remove the shipping cards from inside the drives. Due to the nature of CP/M, turning on the machine with a disk in the drive may result in scrambling the data on the disk - which is why backup disks are a good practice. (Also, you must always remember to take the disks out of the drives before turning off the Omni).

The power switch is a large rocker switch on the rear panel. Turn it on now. The disk drives will start whirring and you will soon see:

* Omni *

Please insert your diskette into Drive A

on the screen.

Put the logic analyzer program disk, the one labeled "Omni Logic Analyzer Operating Disk", in Drive A. It is all right to put a disk in the Omni while the drive is whirring and the red light on the drive is on. (This is not true for all computers). To put the disk in the right way, insert it with the exposed slot to the rear and the label up. Push it in until it clicks in place, then close the door (or actuate the pushbutton or lever). Be careful to avoid bending the disk or touching the brown magnetic surface in the slot, of course.

A.2 MASTER MENU

When you close the door of the drive, the computer will load the CP/M operating system and display the Master Menu. The Master Menu is a new feature that makes the system very easy to use. It displays information about each menu choice automatically.

The Master Menu lists the major disk functions in the left column. For the Logic Analyzer disk, the two major functions listed are:

Logic Analyzer
Disk Utilities

To select a function, use the up-arrow and down-arrow keys to move the darkened area to the function in which you are interested. The text in the right column describes the function marked by the darkened area.

For this example, move the dark area over "Logic Analyzer". Now press the right-arrow key. A sub-menu giving a complete list of the individual functions available will be displayed in the middle column:

Logic Analyzer
EPROM Programmer
Pattern Generator

Again, you can identify the program in which you are most interested by moving the dark area over it. As before, the right column provides details about the marked item.

Select "Logic Analyzer" and press <RETURN>. The Omni will load and begin running the logic analyzer program.

A.3 EARLIER MODELS

Earlier models of the Omni (1984 and prior) do not have the Master Menu feature and use the standard CP/M disk directory user interface. (The standard interface is also available under the Master Menu system; merely press <ESC> to leave the menu and access it.) The logic analyzer functions are the same whether your system has Master Menu or not. If you have the Master Menu feature, skip this section and go to section A.4.

When you close the door of the drive, the computer will load the CP/M operating system from the disk, and respond with the standard prompt:

A0>

Before going further, after the "A0>" prompt type "DIR<RETURN>".

Note: here "<RETURN>" means "press the RETURN key,"
not type the characters "< R E T U R N >".

The directory listing will show at least six files. LA.COM and LA.LAO are the logic analyzer program. LA.LAH contains the Omni's on-line Help

information. DATA-1-.LAD, DATA-2-.LAD, and DATA-S-.LAS contain sample data for this start-up exercise.

When the "A0>" prompt appears again after the directory listing, type "LA<RETURN>". The Omni will load and begin running the logic analyzer program.

A.4 LOGIC ANALYZER PROGRAM

The first part of the logic analyzer program is a self-test sequence. If you have the probes plugged in and connected to nothing, or if there are no probes plugged in, the tests will all be passed and the computer will display

```
CLOCK CIRCUITRY TEST
TRIGGER CONTROL TEST
DATA RAM LOW LEVEL TEST
DATA RAM HIGH LEVEL TEST
GLITCH RAM LOW LEVEL TEST
GLITCH RAM HIGH LEVEL TEST
```

and then go on.

If the probes are plugged in and connected to something, one or more tests will probably fail because the tests assume an "inputs floating" condition. If any test fails, the program will report it and then stop. If necessary, press <SPACE> to override the stop-on-fail and make it go on.

As part of the self-test, the program senses whether inverting or non-inverting probes are connected. The standard Omni probes are inverting type; when no probes are connected, the program interprets that as the non-inverting case. If you plug in the probes after self-test, you must go to the Options Menu and change the Probe Type to Inverting in order to have the data displayed with correct polarity.

A.5 TRIGGER MENU

The first thing that appears after the self-test is the Trigger Setup Menu, which controls the data collection conditions. For example,

```
3) Trigger Event   X X X X X X X X X X X X X X X
```

is the trigger word. Each "X" means "don't care" - trigger with the bit in that position either 0 or 1. An "X" in every position means "trigger on anything."

We will come back to the Trigger Menu shortly. But first, press <SPACE> to access a summary of the available commands. The first page of this listing shows the commands which take parameters, including those which control the Omni's complement of useful displays.

Press any key to access the second page of commands, which lists all the single-stroke commands at your disposal. You can get the command list back on the screen again with the command "?<RETURN>"

anytime the following command prompt line is displayed:

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,(sp),^P

The commands are also listed on the Reference Card following this section, as well as on the keyboard (in abbreviated form). Operation is simple enough, however, that reference to any separate information is unnecessary once you gain a basic familiarity with the machine.

Press <SPACE> to return to the Trigger Menu. Look at Item 1, Active Probes. It has two functions. First, it serves as a logic probe to show the instantaneous logic levels on the input probe lines. Second, it defines the channels that will be included in the Omni's data displays.

The logic probe feature is especially useful because it shows you which lines have activity on them before you try to perform a data collection. Connect the ground clip on one of the probes to a data line and watch the display change.

Practice changing the sampling conditions on the menu. Type "3" to put the cursor on Item 3. Use the left and right arrow keys at the top of the keyboard to move the cursor from bit to bit. Or, press "7" to move the cursor directly to bit 7. Enter a "0" or a "1" in each bit position to specify the trigger word. Use an "X" for "don't care". Press <SPACE> to leave the trigger word.

Ordinarily, after setting up the trigger conditions you would type "G" (for "Go collect data") to tell the machine to collect data, but don't do it now. The trace memory would fill up with all 1's, since the probes "float high" to a 1 level when they are not connected. So instead press <SPACE> once or twice to bring up the Waveform Display.

A.6 WAVEFORM DISPLAY

The Waveform Display has sixteen traces, one for each of the probe data lines. They are labeled DF through DO on the left.

Probably all you will see at this point are flat traces. Near the bottom of the screen is a window that looks like:



The bright area shows where the displayed samples are located in the 1000 samples of data collected. Press the "<" key (or comma, no shift is required). The display will page to the left and you will see some waveforms - actually, meaningless data left in memory from the turn-on sequence. Also observe that the bright area in the window has moved left.

The Waveform Display shows about 80 words out of the Omni's 1000-odd sample memory. The "<" and ">" keys (really, the comma and period) on the keyboard just above the space bar move the display left and right. Try it and see.

A.7 FILES

We also have some sample data stored on disk that you can view.

One of the features that makes the Omni unique in the field of digital analysis is its ability to store sample data and all associated parameters on disk files. Such files appear in the CP/M disk directory with the extension ".LAD".

The LA disk contains a sample file of previously captured data called DATA-1-.LAD. To call it up, type "F" to access the File Menu. Type "4" to access the choice "READ into SAMPLE memory from file". Type "DATA-1-<RETURN>" (do not type ".LAD"; the extension is appended automatically) and the program will load the data.

Now press <SPACE> and notice that the data which was previously on the screen has been replaced by new data.

Study the Waveform Display further; this is a timing display, and it contains a wealth of information. Below the traces is a scale showing the number of each sample in the memory relative to the trigger word. Sample 0 is the trigger word, sample 10 is the tenth after the trigger word, sample -10 is the tenth sample before, and so on.

Below the sample scale is the hex equivalent of each sample word, in the form of four characters in a vertical column.

The highlighted cursor may be moved right or left using the arrow keys at the upper right on the keyboard. Try it. The number and time of the sample marked by the cursor also appear at lower right after "cur:".

Note the prompt line at the bottom of the Waveform Display:

Enter: C,D,E,F,G,H,I,L,M,N,O,P,S,T,W,X,Z,=,?,(sp),^P

This lists the commands that are available. All of the Omni's menus and displays show the available choices at the bottom of the screen. A label on the keyboard also lists these commands.

To call up Help information on the Waveform Display, type "?W" or its lowercase equivalent, "/w".

A.8 DUMP DISPLAY

Next we'll look at a Dump Display of the same data. The Dump Display is the other display most often used along with the Waveform Display. Note which sample the highlighted cursor is on. Type "D<RETURN>" for "Dump".

What you are now seeing is a hex listing of the same data, with the same sample highlighted as before. Use the four cursor keys (top row on the keyboard) to move the cursor around on the screen. As before, the cursor counter "cur:" at the lower right corner gives the number of the marked sample.

A.9 OPTIONS MENU

The number base for the Dump Display is controlled by the Options Menu. Let's change the base and see the same data in binary. Type "O" (the letter "O", not zero) to display the Options Menu. Type "1" to select Item 1 on the menu, Output Number Base.

As soon as you type the "1", the choices available are shown at the bottom of the screen - binary (B), decimal (D), hexadecimal (H), octal (O), and unsigned decimal (U). All the Omni's commands work this way; as soon as you enter the first character, the Omni shows you the format so you can enter the rest of the command correctly. No more hit-or-miss struggling to remember command formats.

Type "B" to change the number base to binary. Now press <SPACE> to return to the Dump Display. Now the same data is displayed in binary.

Before going on, change the base back to hexadecimal. Type "O" to return to the Options Menu again, enter "H" in Item 1, and then press <SPACE> to return to the Dump Display.

The system is designed so that <SPACE> usually takes you to the next page you will need. After viewing a display, <SPACE> takes you to the Trigger Menu so you can change the trigger conditions in preparation for collecting a new sample. Command G then collects the new sample, and displays it in whatever format you used last. If you lose your place, typing <SPACE> once or twice will bring you either the Trigger Menu or an "Enter:" command prompt line. Command T takes you right to the Trigger Menu.

The Omni's flexible data collection - any trigger word or external trigger signal, internal or external clock with trigger and clock qualifiers - coupled with its ability to display the data in many different ways, expands exponentially your ability to collect and interpret meaningful digital data.

A.10 EDGE DISPLAY

Type "E<RETURN>" for Edge Display. Another form of the Waveform Display, the Edge Display emphasizes waveform edges by omitting sequences of 3 or more identical samples. Page the display left and right and note that the long sequences of flat traces you saw in the Waveform Display have been dropped and replaced by vertical rows of blanks. In this case, the Edge Display contains about as much information as three pages of the Waveform Display.

A.11 NAME COMMAND

One of the Omni's most helpful features is the N Command for renaming channels. To rename Channel Zero (the lowest trace), type:

NOTE<RETURN>

which means "name Channel Zero TEST". You will see the label of the lowest trace change to "TEST".

Note that you cannot enter spaces in a label; the space bar is used only to exit the current display. Use underscore characters in place of spaces.

The new channel name automatically carries through to all menus and displays. Press <SPACE> to get back to the Trigger Menu. Type "1" to get on Item 1, then use the cursor key -> repeatedly to step the blinking prompt-cursor along through the channels. The name of whichever channel the prompt-cursor is on will appear at the upper right under "Signal". When you reach channel 0, the name you assigned, "TEST", appears. This feature relieves you of the tedious chore of keeping track of which channel is which, and is one of the benefits of coupling a logic analyzer with a computer.

Press <SPACE> once or twice to leave the Trigger Menu and return to the Edge Display. Note that the program pauses and flashes a "No data has yet been collected" message at the bottom of the screen. This is to warn you that no new data has been collected since you changed a parameter.

A.12 HELP PAGES

Help information is available on-line with a few keystrokes. For example, when viewing a menu, you can call up an explanation of any item by typing "?" followed by the item number. Try it with the Trigger Menu. Type "1" and see the Trigger Menu again. Type "?2" and read an explanation of Item 2, Active Glitch. Press <SPACE> to return to the menu itself, ready to make any changes you want.

Help information is also available on the display commands whenever the cursor-prompt is in the lower left corner of the screen. To get an explanation of any command x, enter "?x". For example, type "?D" to see the Help Pages for the Dump Display and Command. Now go to the Trigger Menu and read the Help Page for each item (1, 2, ... E).

You can print out a complete listing of all the Help Pages on a printer if you wish. Use the command "CTRL-P?" to get the printout.

II. ADVANCED FUNCTIONS

The Omni has six advanced functions - Instruction Disassembly, Signature Analysis, Correlation, Matrix Display, Locate Function, and Histogram Display.

Instruction Disassembly assumes the data in sample memory to be instructions collected from a microprocessor data bus, and translates the data back into microprocessor mnemonics. Signature Analysis calculates signatures from the data in memory. The Correlation Function compares two sets of data, Sample and Reference, to find differences. The Locate Function finds desired data patterns in the sample memory for you. The Histogram Display shows a graph of the percentages of data words lying within consecutive "runs" of varying lengths. The Matrix Display shows the frequency of occurrence of bytes 00 through FF hex within the data sample.

A.13 INSTRUCTION DISASSEMBLY

The default processor for which Instruction Disassembly is performed is the Z80.

Instruction Disassembly is normally used with Channels F-8 connected to a microprocessor data bus. For the Z80, in addition Channels 6 and 7 are connected to the /M1 and /MREQ control signals, which the Omni uses to identify opcode fetches. Channels 5-0 may be used to monitor any other signals you wish - address lines or I/O port bits, for example.

To view a sample of the Omni's Instruction Disassembly capabilities, load the file DATA-2-.LAD into sample memory. Type "F" to access the File Operations Menu, "4", and then "DATA-2-<RETURN>" to read the file. Now type "I-420<RETURN>".

The display you see is somewhat like an assembly listing. On the left side are the bits and bytes, while on the right are the mnemonics and operands. Each line represents one instruction.

For example, if you see "00100001-80", the "00100001" is a binary representation of Channels 7-0, which includes the control lines. "80" is the byte on the data bus (in hexadecimal), and is the opcode for the ADD A,B instruction.

The listing on the right includes not only the mnemonics for the opcodes and operands, but also the hex data corresponding to the execution of the instruction. When a Z80 executes a POP DE instruction, it reads one byte from the program (POP DE is a one-byte instruction), and then reads two more bytes from the stack region of memory for loading into its DE registers. Thus you see these two bytes following the instruction.

Normally you use the microprocessor system memory READ line as the External Clock to collect the sample from the data bus. Collect a

sample with the G Command, then use the I Command to translate it into mnemonics.

Disassembly for the 8085/8080 is performed in a similar manner, using Channels 7, 6, and 5 to sense the 8085/8080 status signals /IOM, S0, and S1.

The Instruction Disassembly function allows you to perform disassembly for other microprocessors by loading the appropriate mnemonics. Mnemonics tables are loaded via Item 2 in the File Menu. A table is currently available for the 8048 family (8748, 80C48, 8039, etc.). You can also create new tables for other processors yourself.

A.14 SIGNATURE ANALYSIS

The next function we'll look at is Signature Analysis, which is controlled by a combined menu and display. Type "S" to call it up.

A "signature" is a kind of checksum calculated from the data stream passing a circuit node. A very powerful troubleshooting technique, signature analysis is used to isolate faults in defective circuit boards. The user compares the signatures of various points on a malfunctioning board to the signatures of the same points on a "known good" board of the same type.

The Omni can collect signatures from up to 14 points at one time. The signatures, which are four-digit hexadecimal numbers, appear in the Sample column on the display. The "known good" signatures (collected previously from a working board and stored on disk) are recalled to appear in the Reference column.

Reference signatures are stored on disk in special files with the extension ".LAS". They must be called up with the Signature Menu, not via the Files Menu like data files.

To call up a sample set of known-good signatures type "7" to put the cursor on Item 7, "Read from file". Then type "DATA-S-", which will load the sample signature file DATA-S-.LAS from disk. (The extension ".LAS" is appended automatically; don't type it.) The stored signatures will then appear in the Reference column.

The G Command tells the Omni to "Go collect a new sample," calculate the signatures, and display them in the Sample column. Any Sample signatures different from the References would be marked by highlighting and a pointer arrow. Having all the Sample and Reference signatures displayed side-by-side makes the comparisons error-free and fast. See the illustration in Section 25 of the manual for an example of the display.

A.15 CORRELATION

The Correlation function allows you to compare two sets of data, one in Sample Memory and the other in Reference Memory. This is useful for comparing questionable data to known good data, or for isolating

small changes in the data that could be nearly impossible to find by eye.

The Reference data may be loaded from a disk file. Type "F" to get the File Menu. Type "3" followed by "DATA-1-<RETURN>" to load the file data into Reference Memory.

Now type "C" to go to the Correlation Menu. Note that "DATA-1-.LAD" appears in Item 1. Press <TAB> to initiate correlation.

Note that this function does not normally perform a new data collection; it merely correlates the data already in Sample Memory to the data in Reference Memory. (An exception: Item 9 on the Correlation Menu allows repeated new data collections and correlations.)

The results of the operation appear as four columns, one sample position in each line. The first column gives the sample number, Sample 0 corresponding to the sample at the trigger event as usual. The second column gives the Sample data. The third column gives the Reference data. The fourth column gives the sample number of the data in Reference Memory. Non-correlating samples are marked by "<=>" and intensified brightness.

A.16 MATRIX DISPLAY

Press <SPACE> to leave Correlation and get the command prompt line.

Type "MALL<RETURN>" to bring up the Matrix Display for samples -488 to 511 (or whatever the trace limits are). The Omni will calculate and display a table giving the number of occurrences of each possible byte (00 through FF) in Sample Memory.

The eight bits on which the Matrix table is based correspond to the eight (or less) lowest active probe lines. (Active probe lines are set on the Trigger Menu, and as of now all sixteen should be active.) The first hex digit of each byte is on the left, the second hex digit on the scale at the top. Look and see how many times the byte "10" occurs.

A.17 LOCATE FUNCTION

We can use the Locate function to find the occurrences of the byte "10" in Sample Memory.

The Locate function is also controlled by a menu; type "L" to bring it up. Item 1, Start Sample Number, contains -488 as the default value so the search will start from the first sample in the data collected. Type "3" to get on the Global Channel Mask item. We want to consider only the lower eight channels in the search, so type "FF<RETURN>" to mask out the upper eight channels. (The Omni will right justify the number entered, so "FF" is the same as "00FF".) Type "4" to get on the Search Pattern item, and then type in "10<RETURN>". Press <SPACE> to leave the Search Pattern items.

Now press <TAB>. The Waveform Display will come back with the first occurrence of "10" marked by the highlighted cursor. If there

were no occurrences, then "Not found" would appear at the upper right on the Locate Menu.

Note that the Locate function does not cause any new data to be collected.

Each time a search pattern is found, the Start Sample Number on the menu will be updated automatically to the start the next at the sample after where the pattern was last found. Once a search pattern has been entered, it is possible to find the second, third, and all subsequent occurrences of the pattern by repeatedly pressing <TAB>.

A.18 HISTOGRAM DISPLAY

The Omni's last function is Histogram, a sophisticated form of statistical analysis. Type "H", which takes you to the Histogram Display. This one combines the menu and display on the same page.

The Histogram is primarily used for studying program execution to improve efficiency. When the data in Sample Memory represents addresses of instructions, the Histogram can be used to measure the amount of time the computer uses executing different parts of the program.

The algorithm that produces the Histogram Display works as follows. It looks through the Sample Memory for sample data falling in the range specified in Items 1 and 2; let us call those "in-range samples." An in-range sample will sometimes appear in a "run" of in-range samples (that is, with other in-range samples before or after it, or both) and sometimes all alone.

Two questions are of interest here. First, how long are the "runs" of in-range samples - how many samples are there in each run? Second, and more important, how are the samples distributed in the runs of different lengths - how many samples fall in short runs versus long runs? So the histogram algorithm identifies the "runs" of in-range samples, sorts them into categories by length of run, and then counts the number of samples in each category.

The column on the left is the run lengths; that is, "5-9" means runs 5 to 9 in-range samples long. The second column is the percentage of in-range samples that fall in runs of varying lengths. The base for the percentage (100%) is the total number of in-range samples in the sample memory. Thus a "7" in the second column next to "5-9" would mean that 7% of the in-range samples fell in runs 5 to 9 samples long.

The Histogram function can perform repeated accumulations for better statistical accuracy.

The Histogram Menu will accept input in other number bases other than hexadecimal. For example, type "1" to put the cursor on Item 1, then type "0<RETURN>" to enter 0. Type "2" to put the cursor on Item 2, then type "999d<RETURN>" to enter 999 decimal. The Omni will calculate and display a histogram based on those values.

A.19 EXITING THE LOGIC ANALYZER PROGRAM

To exit to CP/M, use CTRL-C (press "C" while holding down the <CTRL> key).

A.20 CONCLUSION

Well, that's it. You now know how the Omni works and are ready to hook the probes up to a real circuit and start looking at digital data.

For more detailed study of how to use the Omni's full capability, we suggest you start with Chapter 5 in this manual and read from there.

For your first data collection runs, it's a good idea to use Internal Clock and leave the Trigger Event on the Trigger Menu set to all "don't cares." These conditions will always give you a completed data collection and display any activity on the data lines. Before using External Clock, use this method to check to make sure that the signal you plan to use for the External Clock is actually present.

If the Omni is set to trigger on a certain word and that word is not present in the data stream, triggering will not occur and the machine will just wait. If that happens, press any key except <SPACE> to cause a manual trigger. The data then displayed will be accurate data, however, Sample 0 will correspond to your manual trigger time rather than the trigger word entered on the Trigger Menu. Studying the data will usually give you clues as to why the expected trigger word did not appear.

Rev. D

Appendix B. REFERENCE CARD

<u>Collect or Display Data:</u>		<u>Manual page</u>
D[x]	Numeric dump from sample x	16-1
E[x]	Edge display from sample x	15-1
G	Go and Start Data Collection	12-1
I[x]	Instruction disassembly from sample x	17-1
M[x[,y]]	Matrix display from sample x to y	19-1
W[x[,y]]	Waveform display from sample x to y	13-1
=	Load trigger and collect data	10-3
<u>Utility Commands:</u>		
?[C/D,...]	Help Pages for Commands C, D,...	9-1
N#xyz...	Name Channel number # with xyz...	14-1
CTRL-P[x[,y]]	Print copy of sample x to y	24-1
X[x[,y]]	Calculate time between cursor, x, or y	22-1
<u>Menu Callup Commands:</u>		
C	Correlation Menu	18-1
F	File Operations Menu	20-1
H	Histogram Menu and Display	23-1
L	Locate Pattern Menu	21-1
O	Options Menu	11-1
P	Pattern Generator Menu	30-1
S	Signature Analysis Menu	25-1
T	Trigger Menu	10-1
Z	Multilevel Triggering	29-6
<u>Display Control Keys:</u>		
>	Scroll display to right one page	
<	Scroll display to left one page	
->	Move cursor right one sample	
<-	Move cursor left one sample	
arrow up	Move cursor up one channel or sample	
arrow down	Move cursor down one channel or sample	
<SPACE>	Change mode, terminate function	

This list of the Omni's commands is also on line as two Help Pages. To obtain the first, type "?<RETURN>"; then strike <SPACE> to obtain the second.

Rev. D

OmnLogic, Inc.

LOGIC ANALYZER USER'S COMMENTS

OmnLogic is pleased to receive comments from our users. Problems with either software or the operating manual should be sent to us so that improvements can be made. As these improvements are implemented, software, hardware, and manual updates will be made available to our customers. Please photocopy this form and use it for comments.

Did you find any problems or have any suggestions regarding the hardware?

Did you find any problems or have any suggestions regarding the software?

Did you find the manual understandable, usable, and well-organized? Did you find errors? Please make suggestions for improvement by page number.

Page No. Problem or suggestion

Please indicate how you are using the Omni Logic Analyzer.

Name _____ Date _____

Organization _____ Phone _____

Street _____

City _____ State _____ ZIP _____

Thank you for your help.
OmnLogic, Inc.